



# BEGO IMPLANT SYSTEMS

## Product Catalogue

07/2021

Partners in Progress

**THERE FOR ME.  
BEGO IMPLANT SYSTEMS.**

Dear customers and partners

Teeth are essential for people's well-being – and replacing natural teeth is a major responsibility. For 29 years, this knowledge has motivated us to ensure patients are left feeling comfortable and secure with our implant dentistry solutions.

**How we support you.**

As a family-run company, we put customer proximity and personal cooperation in first place.

With us as a partner by your side, you have access to a comprehensive product range supplemented by the unique Security Implants warranty and our LiVE service program.

Be confident that you can rely on us—always.



## TABLE OF CONTENTS

---

<b>SERVICE</b>	<b>6</b>
BEGO – Solutions from a single source	6
SEMADOS CAMPUS	7
<b>REGENERATION</b>	<b>11</b>
naturesQue Regeneration Line	12
<b>SURGERY</b>	<b>15</b>
Descriptions and labels	16
Implant planning aids	19
BEGO Semados® S implants TG with Platform Switch design	21
BEGO Semados® SC/SCX implants with Platform Switch design	23
BEGO Semados® RS/RSX and RS/RSX <sup>Pro</sup> implants with Platform Switch design	27
BEGO Semados® RI implants with Platform Switch design	31
<b>PROSTHETICS</b>	<b>61</b>
Instruments	62
<b>CAD/CAM Implant Prosthetics BEGO Medical</b>	
• Interface overview	63
• Individual healing abutments	64
• Individual abutments	65
• Occlusally screw-retained bridge restorations	65
• Bar constructions	67
	68
<b>Prosthetics SC/SCX/RS/RSX/RI<sup>*1</sup> implants (PS<sup>*5</sup> design)</b>	
• CAD/CAM restoration	71
• Impression taking and model fabrication	72
• Crown restoration Ø 3.0	75
• Crown and bridge restoration	76
• Multi <sup>Plus</sup> restoration	77
• Hybrid restoration	82
• Screws	86
	89

---

## TABLE OF CONTENTS

---

<b>DEMO MODELS/MATERIAL</b>	<b>109</b>	
Large-scale models	<b>110</b> Demonstration material	<b>111</b>
<b>USEFUL INFORMATION</b>	<b>113</b>	
Torque specifications	<b>114</b> Index by article numbers	<b>122</b>
Material specifications	<b>116</b> Alphabetical index	<b>136</b>

---

**Note:** Depending on regulatory approvals, under some circumstances not all offered products or services are available in all countries.  
Please contact your local BEGO Implant Systems sales partner.

Images and illustrations are examples only and the colors, symbols, design and specifications on the labels and/or packages shown may deviate from real products.

Specifications for lengths and diameters may be rounded up or down for simplification.

Our products are constantly being refined. We therefore reserve the right to make changes.

© 2021 by BEGO Implant Systems GmbH & Co. KG, Bremen. We reserve all rights to reprints of extracts, photomechanical reproduction and particularly translations.

\*<sup>1</sup> Version of the BEGO Semados® RI implants with platform switch design

\*<sup>2</sup> Platform Switch design

\*<sup>7</sup> Platform Match design

## Solutions from a single source



### Conventional solutions

BEGO Bremer Goldschägerei GmbH & Co. KG develops and sells precious metal and non-precious metal dental alloys and provides equipment, materials and services for fabricating premium dental restorations. The company also offers ceramics for further processing in the dental laboratory. Since its founding, and now moving into its fifth generation, BEGO has realized its aim of providing dental laboratories with innovative and cost-effect products and services for optimal treatment of their patients, all from a single source.



### CAD/CAM solutions

BEGO Medical GmbH specializes in digital processes and is a pioneer in CAD/CAM technology in the dental sector. The company is the inventor and holder of the patent for the Selective Laser Melting (SLM) procedure in the dental sector. All-round procedural expertise and the widest choice of materials ensure premium quality across many indications. In its high-tech production centre located in Bremen, BEGO fabricates frameworks, abutments, crowns and bridges based on virtual models using the latest laser and milling techniques in four different procedures: SLM, High Speed Cutting (HSC), CAD/Cast® and Rapid Prototyping.

### Implant dentistry solutions

Since 1990 BEGO Implant Systems GmbH & Co. KG has been developing and fabricating dental implants and supplementary products to treat patients with implants around the world. An innovative 3D implant design, system abutments for modern implant dentistry, a safe biomaterials system, and functionally optimized guided surgery all mean that dental implants "Made by BEGO" lead to planned and reproducible results. These are premium German products that incorporate technological progress with fair prices, combining safety, durability, aesthetics and reliability.



### BEGO TRAINING CENTER

Practical knowledge of subjects such as CAD/CAM or traditional dental technology are taught by an internationally experienced team of trainers in courses – both for beginners and advanced users – that are specifically tailored to meet the most diverse requirements.

Our in-house course concepts form the basis of a challenging program for seminars and practical courses that help motivated dental technicians become even more successful.

## **Professional development: A focus of BEGO Implant Systems SEMA DOS CAMPUS**

Supporting postgraduate dental training and qualification of dental technicians in the area of modern, implant-retained prosthetics is the focus of BEGO Implant Systems – and has been right from the start.

So that we can continuously optimize our training programs, we have formed a number of framework agreements with various national and international professional development training centres under the umbrella brand SEMADOS CAMPUS. You can read about our international training programs in our course brochure. Our website also has more information about the latest courses on offer.

For international training programs, please contact our worldwide sales partners or contact BEGO Implant Systems in Bremen directly.

For professional development courses for dental technicians, the BEGO TRAINING CENTER <https://www.bego.com/courses-events/education/bego-training-center/> in Bremen is available.

Is there a course or training program you'd like to see offered? We happily accept any suggestions you may have.

# SEMA DOS Campus

# BEGO IMPLANT OVERVIEW

Those who want to treat their patients based on needs require comprehensive treatment solutions. Our implant systems are highly suited for many areas of application.

## Parallel implant shape

..... Self-tapping .....



## Conical implant shape

Self-tapping .....



Condensing .....



The implants have a conical inner connection with a mean conical angle of 45° as well as an internal hex that acts as an anti-rotation mechanism.



### The choice is yours

Tailored to your patient down to the finest detail – BEGO Semados® S-TG/S/SC/SCX

#### S implant TG

- Implant interface at gingival height
- High machined implant shoulder
- One-stage implantation technique is possible
- Platform Switch design

#### S implant

- Increase in the primary stability thanks to increasing core diameter with decreasing thread depth
- Platform Match design
- Fully guided surgery is an option

#### SC/SCX implant

- Preservation of the crestal bone thanks to the integrated Platform Switch
- Machined or micro-structured implant shoulder
- Fully guided surgery is an option

### Fits just about every time

Depending on preference – BEGO Semados® RS/RSX or RS/RSX<sup>Pro</sup>

#### RS/RSX implant 3.0

- For narrow anterior gaps to replace teeth 12, 22, 32–42
- Just a few rotations needed when inserting
- Platform Switch design
- Fully guided surgery is an option

#### RS/RSX<sup>Pro</sup> implant

- Low stresses in the implant—self-tapping bionic thread designed to withstand stresses
- Diameter 5.5 available in a length of 7 mm
- Platform Switch design

- Fully guided surgery is an option

### Cuts a really fine figure

For primary and long-term stability – BEGO Semados® RI

#### RI implant

- Microthread in the neck region—for improved force transfer to the crestal bone
- Increase in the primary stability due to the condensing thread design for lateral bone condensation
- Platform Switch design
- Optional guided pilot drill hole

### For all requirements

Classic or compact – BEGO Semados® Tray

Our plastic trays without separate silicone stoppers ensure cleaning with a consistently high and verifiable quality.

A clearly arranged instrument set and a color-coding system for an easy and safe workflow.

## Safe and simple. Comprehensive and guaranteed: BEGO SECURITY Implants



BEGO has been active in the dentistry sector since 1890 and has in-house research and development units and production and quality assurance processes to ensure that the stringent requirements for medical devices are satisfied. The tolerability of BEGO materials is also verified by independent institutes. Place your trust in the BEGO brand and make the most of our warranty agreements. Actively support the selling of your high-quality work. Offer your patients additional security when choosing a recommended restoration. Patients can expect out-of-pocket costs for premium restorations and place high expectations on the quality and longevity of their restoration.

Implant dentistry restorations with BEGO Semados® implants can be provided with warranty coverage of 60 months, that is, 5 years, from the day of implantation by implant dentists using BEGO SECURITY Implants. This is a true added value for premium restorations, giving patients additional security.

More information is available here:



BEGO Implant Systems provides a patient passport that includes information for patients and documentation of the restoration.

### BEGO SECURITY Implants— Your benefits \*<sup>E</sup> at a glance:

- replaces dentistry fees, laboratory and material costs
- no contractual obligation required
- low administrative effort
- low costs
- 60 months (5 years) warranty from implantation
- covers restorations with BEGO Semados® implants, their prosthetic components, and prosthetic supraconstructions fabricated in BEGO CAD / CAM processes
- also applies for prosthetic restorations

\*<sup>E</sup> All information applies under consideration of the particular warranty conditions.  
(BEGO SECURITY Implants Product Information, REF 83528)

<sup>4</sup> Please take into consideration the particular warranty conditions in the BEGO SECURITY implants product information, REF 83528. May not be available in all countries.



## OVERVIEW

naturesQue Regeneration Line

12

naturesQue Regeneration Line					
Description	REF	Specification	Container	Contents	
<b>naturesQue MaxOss P</b> porcine bone substitute material	58488	0.25–1.0mm	Jar	0.5ml	
	58489	0.25–1.0mm	Jar	1.0ml	
	58490	0.25–1.0mm	Jar	2.0ml	
	58491	0.25–1.0mm	Jar	4.0ml	
	58492	1.0–2.0mm	Jar	1.0ml	
	58493	1.0–2.0mm	Jar	2.0ml	
	58494	0.25–1.0mm	Syringe	0.25ml	
	58495	0.25–1.0mm	Syringe	0.5ml	
<b>naturesQue SemOss B</b> Xenohybrid bovine bone substitute material	58500	0.25–1.0mm	Vial	0.25g; 0.5ml	
	58501	0.25–1.0mm	Vial	0.5g; 1.0ml	
	58502	0.25–1.0mm	Vial	1.0g; 2.0ml	
	58503	0.25–1.0mm	Vial	2.0g; 4.0ml	
	58504	1.0–2.0mm	Vial	0.5g; 1.0ml	
	58505	1.0–2.0mm	Vial	1.0g; 2.0ml	
	58506	1.0–2.0mm	Vial	2.0g; 4.0ml	
<b>naturesQue ColTect P</b> porcine barrier membrane	58496	15 × 20mm	Piece	1	
	58497	20 × 30mm	Piece	1	
	58498	30 × 40mm	Piece	1	
<b>naturesQue ColAid B</b> bovine collagen microfibrils	58499	0.1g	Vial	15	
<b>naturesQue ColAid P</b> porcine collagen fleece	58507	20 × 20mm	Piece	10	

**Note:** Depending on regulatory approvals, not all naturesQue products are available in all countries.  
Please contact your local BEGO Implant Systems sales partner.  
Returns and exchanges are not possible because of the temperature sensitivity of these products.

[Duck]  
synonymous with empathy,  
trust, and respect

# naturesQue

»  
**REGENERATION  
MATERIALS**



naturesQue Regeneration Materials  
combines the strengths of the  
products' natural origins with  
scientific and clinical expertise for  
tissue regeneration.

## The essence of nature in expert hands.

**BEGO IMPLANT SYSTEMS**

Partners in Progress

[www.bego.com](http://www.bego.com)

 BEGO





## OVERVIEW

Descriptions and labels	16
Implant planning aids	19
BEGO Semados® S implants TG with Platform Switch design	21
BEGO Semados® SC/SCX implants with Platform Switch design	23
BEGO Semados® RS/RSX and RS/RSX <sup>Pro</sup> implants with Platform Switch design	27
BEGO Semados® RI implants with Platform Switch design	31
Cover screws/healing abutments with Platform Switch design	33
BEGO Semados® S implants with Platform Match design	37
Cover screws/healing abutments with Platform Match design	39
BEGO Guide guided surgery	41
Preparation instruments	49

## Platform Switch



## Platform Match



## The BEGO Semados® implant family

### Platform Switch implants

#### S implant TG

Transgingival, self-tapping, cylindrical implant with 3 mm machined implant shoulder

#### SC implant

self-tapping, cylindrical implant with 0.5mm machined implant shoulder

#### SCX implant

self-tapping, cylindrical implant with 0.1mm machined implant shoulder

#### RS implant

self-tapping, conical implant with 0.5mm machined implant shoulder

#### RSX implant

self-tapping, conical implant with 0.1mm machined implant shoulder

#### RI implant

self-condensing, conical implant with 0.5mm machined implant shoulder

### Platform Match Implant

#### S implant

self-tapping, cylindrical implant with 0.8mm machined implant shoulder

### Color coding/diameter

BEGO Semados® RS/RSX implant

3.0



BEGO Semados® S/SC/SCX implant

3.25



BEGO Semados® S/SC/SCX/RS/RSX/RI implant

3.75



BEGO Semados® S/SC/SCX/RS/RSX/RI implant

4.1



BEGO Semados® S/SC/SCX/RS/RSX/RI implant

4.5



BEGO Semados® S/SC/SCX/RS/RSX/RI implant


5.5




**Note:** BEGO Semados® S/SC/SCX implant 3.25–4.5 and RS/RSX implant 3.0–4.5, template-guided preparation using the BEGO Guide System is an option.

## Label and sticker

- |        |   |  |
|--------|---|--|
| 1      |    | Manufacturer   |
| 2      |   | Article description/size information   |
| 3      |   | <b>Color coding</b><br><input type="checkbox"/> Ø 3.0 <input checked="" type="checkbox"/> Ø 3.25 <input type="checkbox"/> Ø 3.75 <input type="checkbox"/> Ø 4.1 <input checked="" type="checkbox"/> Ø 4.5 <input type="checkbox"/> Ø 5.5 |
|        |    | <b>Article number</b>  |
|        |    | <b>Batch code</b>  |
|        |    | <b>Quantity</b>  |
|        |    | <b>Data Matrix Code</b>  |
|        |    | Includes manufacturer and article number.<br>If necessary, also batch number and/<br>or expiry date  |
| 4      |   | <b>Product description</b>   |
| 5      |  | <b>Use by</b>  |
|        |  | <b>CE marking</b>  |
|        |  | <b>Do not reuse</b>  |
|        |  | <b>Sterilized using irradiation</b>  |
|        |  | <b>Do not resterilize</b>  |
|        |  | <b>Non-sterile</b>   |
|        |  | <b>Consult instructions for use<br/>for electronic instructions for use</b><br>ifu.bego.com  |
|        |  | <b>Do not use if package is damaged</b>  |
|        |  | <b>Caution</b>   |
|        |  | <b>Temperature limit</b>   |
|        |  | <b>Keep away from sunlight</b>   |
| RxOnly |   | According to US Federal law, this product may only be sold to trained physicians or on their behalf  |
|        |  | <b>Speed of rotation</b>   |
|        |  | <b>Packaging system comprising non-sterile protective packaging and a sterile barrier system</b>   |
|        |  | <b>Medical device</b>  |
|        |  | <b>MR conditional</b>  |
| 6      |  | <b>Product model</b>   |
|        |  | <b>Information website for patients</b>  |

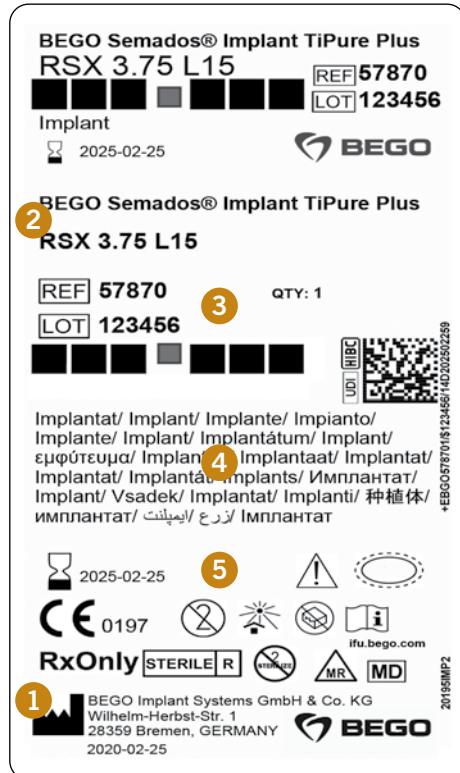

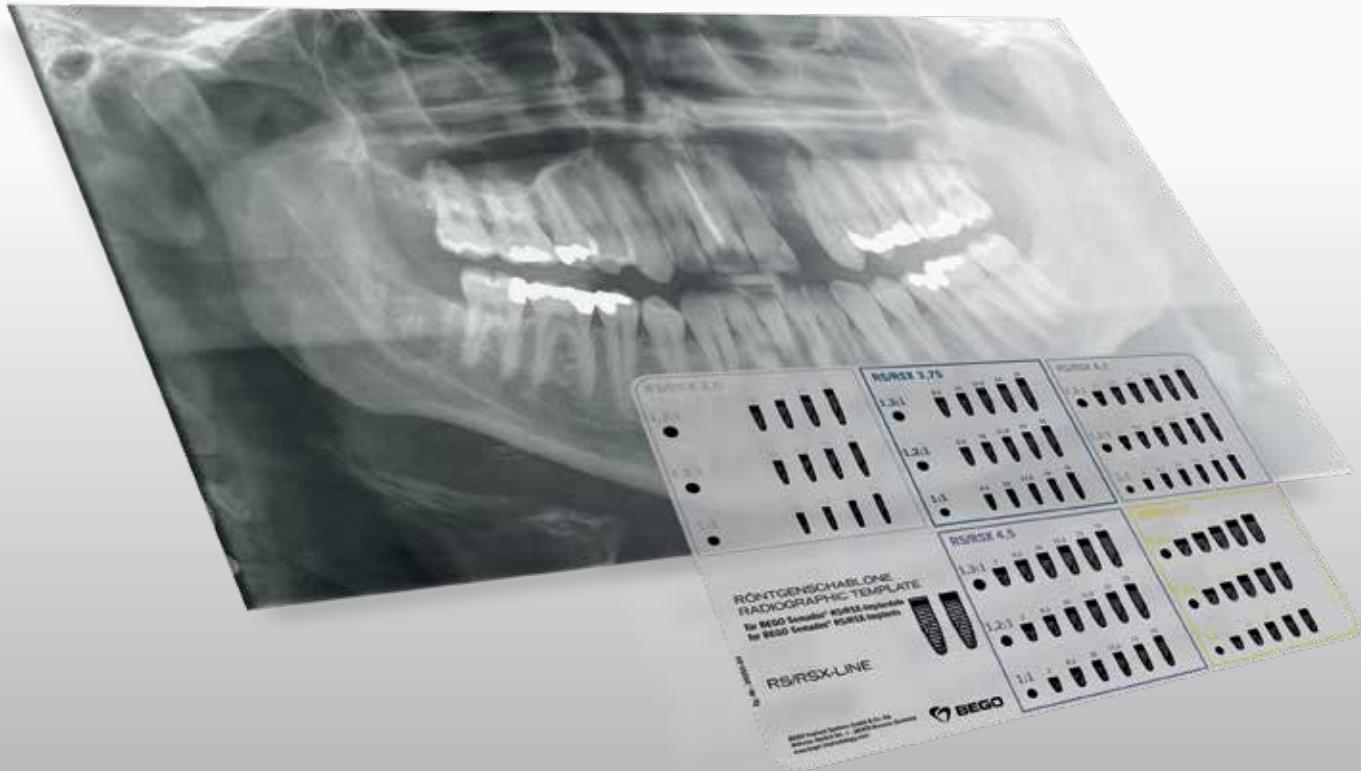

## OVERVIEW

Radiographic templates

20

Radiographic templates					
Description	REF	Color code	Size	Compatibility	Units
Radiographic templates	53888			S implants	1
	58246			SC/SCX implants	1
	57959			RS/RSX implants	1
	55745			RI implants	1





## SOMETIMES SIZE MATTERS

### Your benefits

- Implant interface at gingival height
- High machined implant shoulder
- One-stage implantation technique is possible
- For the most stringent quality requirements—100% German development and manufacturing
- Same implant–abutment interface as for BEGO Semados® SC/SCX/RS/RSX implant systems
- Stable connection with no micro-movements during functional masticatory loading (up to 150 N)
- Use in combination with BEGO Semados® S-Line Tray<sup>Plus</sup>

### Technical details


- Self-tapping implant with Platform Switch and 3 mm machined implant shoulder
- Diameter: 3.75 · 4.1 mm
- Lengths: 10 · 13 mm (osseous nominal size + gingival area)
- Gap-free fit of the abutments thanks to the internal taper
- Manufactured from grade 4 pure titanium with ultrapure homogeneous TiPure<sup>Plus</sup> surface




Consult instructions for use

## SURGERY · S IMPLANTS TG WITH PS<sup>\*5</sup> DESIGN

Implants					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Semados® implants</b> incl. cover screw and titanium insertion posts TiPure <sup>Plus</sup> surface Material: Titanium grade 4 (packaged sterile)	58330	■	3,75 L10	S-TG (PS)	1
	58331	■	3,75 L13	S-TG (PS)	1
	58333	■	4,1 L10	S-TG (PS)	1
	58334	■	4,1 L13	S-TG (PS)	1
					
<b>BEGO SECURITY implants<sup>*4</sup></b> Implant warranty	83538				1
					

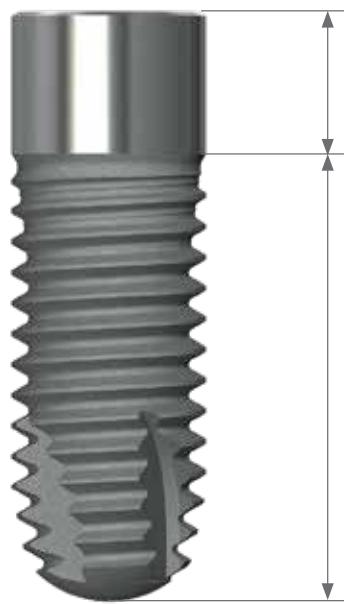

S implant TG L10, total length 12.5 mm

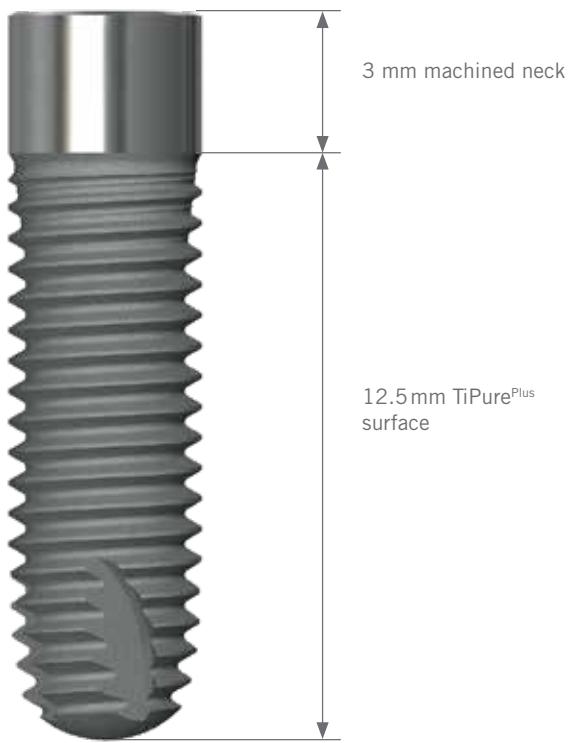

S implant TG L13, total length 15.5 mm

### Note:

- TG = Transgingival
- Preparation corresponding to the stated nominal lengths (L10 or L13)
- Compatible with existing Platform Switch prostheses (PS Line)

<sup>\*4</sup> Please take into consideration the particular warranty conditions in the BEGO SECURITY implants product information, REF 83528. May not be available in all countries.  
<sup>\*5</sup> Platform Switch Design.



## YOU HAVE THE CHOICE

### Your benefits

- SC/SCX implants – preservation of the crestal bone thanks to the integrated Platform Switch
- Efficient – just one surgical tray needed
- Well thought out – cover screw included
- Freedom of choice based on preference and indication – machined implant shoulder (SC implants) or micro-structured (SCX implants)
- Optional – Navigated/template-guided preparation of the BEGO Semados® SC/SCX implants with diameters 3.25–4.5 using the BEGO Guide system
- To satisfy the most stringent quality requirements – 100% German development and production

### Technical details

- Platform Switch
- Gap-free fit of the abutments thanks to the internal taper
- Self-tapping thread
- Manufactured from grade 4 pure titanium with ultrapure homogeneous TiPurePlus surface
- Diameter: 3.25 · 3.75 · 4.1 · 4.5 · 5.5mm
- Lengths: 7 · 8.5 · 10 · 11.5 · 13 · 15mm
- Diameter 5.5mm in length 7mm if there is not much vertical bone height available



Consult instructions for use

## SURGERY · SC/SCX IMPLANTS WITH PS<sup>\*5</sup> DESIGN

Implants					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Semados® implants</b> incl. cover screw and titanium insertion post TiPure <sup>Plus</sup> surface Material: Titanium grade 4 (packaged sterile)	58160	■	3.25 L8.5	SC	1
	58161	■	3.25 L10	SC	1
	58162	■	3.25 L11.5	SC	1
	58163	■	3.25 L13	SC	1
	58164	■	3.25 L15	SC	1
	58165	■■	3.75 L8.5	SC	1
	58166	■■	3.75 L10	SC	1
	58167	■■	3.75 L11.5	SC	1
	58168	■■	3.75 L13	SC	1
	58169	■■	3.75 L15	SC	1
	58170	■■■	4.1 L7	SC	1
	58171	■■■	4.1 L8.5	SC	1
	58172	■■■	4.1 L10	SC	1
	58173	■■■	4.1 L11.5	SC	1
	58174	■■■	4.1 L13	SC	1
	58175	■■■	4.1 L15	SC	1
	58176	■■■■	4.5 L7	SC	1
	58177	■■■■	4.5 L8.5	SC	1
	58178	■■■■	4.5 L10	SC	1
	58179	■■■■	4.5 L11.5	SC	1
	58180	■■■■	4.5 L13	SC	1
	58181	■■■■	4.5 L15	SC	1
	58182	■■■■■	5.5 L7	SC	1
	58183	■■■■■	5.5 L8.5	SC	1
	58184	■■■■■	5.5 L10	SC	1
	58185	■■■■■	5.5 L11.5	SC	1
	58186	■■■■■	5.5 L13	SC	1

**Note:** BEGO Semados® SC/SCX implants 3.25–4.5, template-guided preparation using the BEGO Guide System is an option.

\*5 Platform Switch Design

## SURGERY · SC/SCX IMPLANTS WITH PS\*<sup>5</sup> DESIGN

Implants					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Semados® implants</b> incl. cover screw and titanium insertion posts TiPure <sup>Plus</sup> surface Material: Titanium grade 4 (packaged sterile)	58260	■	3.25 L8.5	SCX	1
	58261	■	3.25 L10	SCX	1
	58262	■	3.25 L11.5	SCX	1
	58263	■	3.25 L13	SCX	1
	58264	■	3.25 L15	SCX	1
	58265	■■	3.75 L8.5	SCX	1
	58266	■■	3.75 L10	SCX	1
	58267	■■	3.75 L11.5	SCX	1
	58268	■■	3.75 L13	SCX	1
	58269	■■	3.75 L15	SCX	1
	58270	■■	4.1 L7	SCX	1
	58271	■■	4.1 L8.5	SCX	1
	58272	■■	4.1 L10	SCX	1
	58273	■■	4.1 L11.5	SCX	1
	58274	■■	4.1 L13	SCX	1
	58275	■■	4.1 L15	SCX	1
	58276	■■■	4.5 L7	SCX	1
	58277	■■■	4.5 L8.5	SCX	1
	58278	■■■	4.5 L10	SCX	1
	58279	■■■	4.5 L11.5	SCX	1
	58280	■■■	4.5 L13	SCX	1
	58281	■■■	4.5 L15	SCX	1
	58282	■■■■	5.5 L7	SCX	1
	58283	■■■■	5.5 L8.5	SCX	1
	58284	■■■■	5.5 L10	SCX	1
	58285	■■■■	5.5 L11.5	SCX	1
	58286	■■■■	5.5 L13	SCX	1

Watch the video “BEGO Semados® SC/SCX implant”:



## SURGERY · SC/SCX IMPLANTS WITH PS<sup>\*5</sup> DESIGN

Implants					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO SECURITY implants<sup>*4</sup></b> Implant warranty	83538				1



<sup>\*4</sup> Please take into consideration the particular warranty conditions in the BEGO SECURITY implants product information, REF 83528. May not be available in all countries.



## FITS JUST ABOUT EVERY TIME

### Your benefits

- Low stresses in the implant—self-tapping bionic thread designed to withstand stresses
- Integrated platform switching—supports the preservation of crestal bone
- Fast—only a few rotations needed for insertion
- Simple to use—inserting using self-centering
- Well thought out—cover screw included
- Optional—navigated/template-guided preparation of the implants with diameters 3.0–4.5 using the BEGO Guide system
- For the most stringent quality requirements—100% German development and manufacturing

### Technical details

- Conical implant shape with rounded apex
- Self-tapping thread design with optimal cutting angle
- Diameter: 3.0 · 3.75 · 4.1 · 4.5 · 5.5 mm
- Lengths: 7 · 8.5 · 10 · 11.5 · 13 · 15 mm
- Fabricated from grade 4 pure titanium with TiPure<sup>Plus</sup> surface
- Gap-free fit of the abutments thanks to the internal taper
- RS/RSX 3.0 suitable for use with narrow anterior gaps
- to replace teeth 12, 22, 32–42
- Diameter 5.5 in length 7 mm, for cases without appropriate vertical bone height available



Consult instructions for use

Implants					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Semados® implants</b> incl. cover screw and titanium insertion posts TiPure <sup>Plus</sup> surface Material: Titanium grade 4 (packaged sterile)	57962	□	3.0 L10	RS	1
	57963	□	3.0 L11.5	RS	1
	57964	□	3.0 L13	RS	1
	58966	■	3.75 L8.5	RS <sup>Pro</sup>	1
	58967	■	3.75 L10	RS <sup>Pro</sup>	1
	58968	■	3.75 L11.5	RS <sup>Pro</sup>	1
	58969	■	3.75 L13	RS <sup>Pro</sup>	1
	58970	■	3.75 L15	RS <sup>Pro</sup>	1
	58971	■	4.1 L7	RS <sup>Pro</sup>	1
	58972	■	4.1 L8.5	RS <sup>Pro</sup>	1
	58973	■	4.1 L10	RS <sup>Pro</sup>	1
	58974	■	4.1 L11.5	RS <sup>Pro</sup>	1
	58975	■	4.1 L13	RS <sup>Pro</sup>	1
	58976	■	4.1 L15	RS <sup>Pro</sup>	1
	58977	■	4.5 L7	RS <sup>Pro</sup>	1
	58978	■	4.5 L8.5	RS <sup>Pro</sup>	1
	58979	■	4.5 L10	RS <sup>Pro</sup>	1
	58980	■	4.5 L11.5	RS <sup>Pro</sup>	1
	58981	■	4.5 L13	RS <sup>Pro</sup>	1
	58982	■	4.5 L15	RS <sup>Pro</sup>	1
	58983	■	5.5 L7	RS <sup>Pro</sup>	1
	58984	■	5.5 L8.5	RS <sup>Pro</sup>	1
	58985	■	5.5 L10	RS <sup>Pro</sup>	1
	58986	■	5.5 L11.5	RS <sup>Pro</sup>	1
	58987	■	5.5 L13	RS <sup>Pro</sup>	1

**Note:** BEGO Semados® RS/RSX and RS/RSX<sup>Pro</sup>-implants 3.0–4.5, template-guided preparation using the BEGO Guide System is an option.

\*<sup>5</sup> Platform Switch design

Implants					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Semados® implants</b> incl. cover screw and titanium insertion posts TiPure <sup>Plus</sup> surface Material: Titanium grade 4 (packaged sterile)	57862	□	3.0 L10	RSX	1
	57863	□	3.0 L11.5	RSX	1
	57864	□	3.0 L13	RSX	1
	58866	■	3.75 L8.5	RSX <sup>Pro</sup>	1
	58867	■	3.75 L10	RSX <sup>Pro</sup>	1
	58868	■	3.75 L11.5	RSX <sup>Pro</sup>	1
	58869	■	3.75 L13	RSX <sup>Pro</sup>	1
	58870	■	3.75 L15	RSX <sup>Pro</sup>	1
	58871	■	4.1 L7	RSX <sup>Pro</sup>	1
	58872	■	4.1 L8.5	RSX <sup>Pro</sup>	1
	58873	■	4.1 L10	RSX <sup>Pro</sup>	1
	58874	■	4.1 L11.5	RSX <sup>Pro</sup>	1
	58875	■	4.1 L13	RSX <sup>Pro</sup>	1
	58876	■	4.1 L15	RSX <sup>Pro</sup>	1
	58877	■	4.5 L7	RSX <sup>Pro</sup>	1
	58878	■	4.5 L8.5	RSX <sup>Pro</sup>	1
	58879	■	4.5 L10	RSX <sup>Pro</sup>	1
	58880	■	4.5 L11.5	RSX <sup>Pro</sup>	1
	58881	■	4.5 L13	RSX <sup>Pro</sup>	1
	58882	■	4.5 L15	RSX <sup>Pro</sup>	1
	58883	■	5.5 L7	RSX <sup>Pro</sup>	1
	58884	■	5.5 L8.5	RSX <sup>Pro</sup>	1
	58885	■	5.5 L10	RSX <sup>Pro</sup>	1
	58886	■	5.5 L11.5	RSX <sup>Pro</sup>	1
	58887	■	5.5 L13	RSX <sup>Pro</sup>	1

Watch the video "BEGO Semados® RS/RSX and RS/RSX<sup>Pro</sup>-implant":



Implants					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO SECURITY implants<sup>*4</sup></b> Implant warranty	83538				1



<sup>\*4</sup> Please take into consideration the particular warranty conditions in the BEGO SECURITY implants product information, REF 83528. May not be available in all countries.

<sup>\*5</sup> Platform Switch design



## CUTS A FINE FIGURE

### Your benefits

- Microthread in the neck region – for improved force transfer to the crestal bone
- Increase in the primary stability due to the condensing thread design for lateral bone compression
- Well thought out – cover screw included
- Integrated Platform Switch supports the preservation of the crestal bone
- To satisfy the most stringent quality requirements – 100% German development and production
- Stable connection with no micro-movements during functional masticatory loading (up to 150N)

### Technical details

- Self-condensing, conical implant with Platform Switch and 0.5mm machined implant shoulder
- Diameter: 3.75 · 4.1 · 4.5 · 5.5mm
- Lengths: 8.5 · 10 · 11.5 · 13mm
- Manufactured from grade 4 pure titanium with ultrapure homogeneous TiPure<sup>Plus</sup> surface
- Gap-free fit of the abutments thanks to the internal taper
- Internal hex prevents rotation of abutments



Consult instructions for use

## SURGERY · RI IMPLANTS WITH PS<sup>\*5</sup> DESIGN

Implants					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Semados® implants</b> incl. cover screw and titanium insertion posts TiPure <sup>Plus</sup> surface Material: Titanium grade 4 (packaged sterile)	57708	■	3.75 L8.5	RI*1	1
	57709	■	3.75 L10	RI*1	1
	57710	■	3.75 L11.5	RI*1	1
	57711	■	3.75 L13	RI*1	1
	57718	■	4.1 L8.5	RI*1	1
	57719	■	4.1 L10	RI*1	1
	57720	■	4.1 L11.5	RI*1	1
	57721	■	4.1 L13	RI*1	1
	57728	■	4.5 L8.5	RI*1	1
	57729	■	4.5 L10	RI*1	1
	57730	■	4.5 L11.5	RI*1	1
	57731	■	4.5 L13	RI*1	1
	57738	■	5.5 L8.5	RI*1	1
	57739	■	5.5 L10	RI*1	1
	57740	■	5.5 L11.5	RI*1	1
	57741	■	5.5 L13	RI*1	1
<b>BEGO SECURITY implants<sup>*4</sup></b> Implant warranty	83538				1

Watch the video “BEGO Semados® RI implant”:



\*1 Version of the BEGO Semados® RI implants with platform switch design  
 \*4 Please take into consideration the particular warranty conditions in the BEGO SECURITY implants product information, REF 83528. May not be available in all countries.  
 \*5 Platform Switch design



## OVERVIEW

Cover screws	34
Healing abutments	34

## SURGERY · COVER SCREWS/HEALING ABUTMENTS WITH PS<sup>\*5</sup> DESIGN

### Cover screws

Description	REF	Color code	Size	Compatibility	Units
<b>Implant cover screws</b>					
Material: Titanium grade 4 (packaged sterile)	57950	□		RS/RSX 3.0	1
Tool: Hexagon screwdriver 1.25mm *2	58290	■		SC/SCX 3.25	1
	57951	■■		SC/SCX/RS/RSX/RI*1 3.75	1
	57952	■■■		SC/SCX/RS/RSX/RI*1 4.1	1
	57953	■■■■		SC/SCX/RS/RSX/RI*1 4.5	1
	57954	■■■■■		SC/SCX/RS/RSX/RI*1 5.5	1



### Healing abutments

Description	REF	Color code	Size	Compatibility	Units
<b>PS HP</b>					
prefabricated gingival former	57764	□	Ø3.0 L3	RS/RSX 3.0	1
Material: Titanium alloy (packaged sterile)	57765	□	Ø3.0 L5	RS/RSX 3.0	1
Tool: Hexagon screwdriver 1.25mm/slot screwdriver *2	57766	□	Ø3.0 L7	RS/RSX 3.0	1
	57767	□	Ø4.0 L3	RS/RSX 3.0	1
	57768	□	Ø4.0 L5	RS/RSX 3.0	1
	57769	□	Ø4.0 L7	RS/RSX 3.0	1
<b>Implant diameter 3.0</b>					
	57807	■■	Ø4.5 L3	SC/SCX/RS/RSX/RI*1 3.25–3.75	1
	57808	■■	Ø4.5 L5	SC/SCX/RS/RSX/RI*1 3.25–3.75	1
	58150	■■	Ø4.5 L7	SC/SCX/RS/RSX/RI*1 3.25–3.75	1
<b>Implant diameter 3.25–3.75</b>					
	57809	■■■	Ø5.0 L3	SC/SCX/RS/RSX/RI*1 4.1	1
	57810	■■■	Ø5.0 L5	SC/SCX/RS/RSX/RI*1 4.1	1
	58151	■■■	Ø5.0 L7	SC/SCX/RS/RSX/RI*1 4.1	1
<b>Implant diameter 4.1</b>					
	57811	■■■■	Ø5.5 L3	SC/SCX/RS/RSX/RI*1 4.5	1
	57812	■■■■	Ø5.5 L5	SC/SCX/RS/RSX/RI*1 4.5	1
	58152	■■■■	Ø5.5 L7	SC/SCX/RS/RSX/RI*1 4.5	1
<b>Implant diameter 4.5</b>					
	57813	■■■■■	Ø6.5 L3	SC/SCX/RS/RSX/RI*1 5.5	1
	57814	■■■■■	Ø6.5 L5	SC/SCX/RS/RSX/RI*1 5.5	1
	58153	■■■■■	Ø6.5 L7	SC/SCX/RS/RSX/RI*1 5.5	1



\*1 Version of the BEGO Semados® RI implants, with Platform Switch design

\*2 For torque specifications, see page 114

\*5 Platform Switch design

Healing abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>PS HPW</b> prefabricated gingival former Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25mm/slot screwdriver *2	<b>Implant diameter 3.25–3.75</b>				
	57815	■■	Ø 5.5 L3	SC/SCX/RS/RSX/RI <sup>*1</sup>	3.25–3.75
	58200	■■	Ø 5.5 L5	SC/SCX/RS/RSX/RI <sup>*1</sup>	3.25–3.75
	58201	■■	Ø 5.5 L7	SC/SCX/RS/RSX/RI <sup>*1</sup>	3.25–3.75
	<b>Implant diameter 4.1</b>				
	57816	■	Ø 6.0 L3	SC/SCX/RS/RSX/RI <sup>*1</sup>	4.1
	58202	■	Ø 6.0 L5	SC/SCX/RS/RSX/RI <sup>*1</sup>	4.1
	58203	■	Ø 6.0 L7	SC/SCX/RS/RSX/RI <sup>*1</sup>	4.1
	<b>Implant diameter 4.5</b>				
	57817	■	Ø 6.5 L3	SC/SCX/RS/RSX/RI <sup>*1</sup>	4.5
	58204	■	Ø 6.5 L5	SC/SCX/RS/RSX/RI <sup>*1</sup>	4.5
	58205	■	Ø 6.5 L7	SC/SCX/RS/RSX/RI <sup>*1</sup>	4.5
	<b>Implant diameter 5.5</b>				
	57818	■	Ø 7.0 L3	SC/SCX/RS/RSX/RI <sup>*1</sup>	5.5
	58206	■	Ø 7.0 L5	SC/SCX/RS/RSX/RI <sup>*1</sup>	5.5



Healing abutment					
Description	REF	Color code	Size	Compatibility	Units
<b>Healing abutment, individual</b> customisable gingival former comprising: • healing abutment • prosthesis screw Hex 1.25mm Material: Polyetheretherketone (PEEK) Tool: Hexagon screwdriver 1.25mm *2	55953	■■■■■	Ø 7.0	S/SC/SCX/RS/RSX/RI	3.25–5.5



---

<sup>\*7</sup> Platform Match design



## YOUR TRIED-AND-TESTED SYSTEM – FAMILIAR YET NEW

### Your benefits

- S implants – increase in the primary stability thanks to increasing core diameter with decreasing thread depth
- Machined implant shoulder
- Well thought out – cover screw included
- Optional – Navigated/template-guided preparation of the BEGO Semados® S implants with diameters 3.25–4.5 using the BEGO Guide system
- To satisfy the most stringent quality requirements – 100% German development and production

### Technical details

- Platform Match
- Gap-free fit of the abutments thanks to the internal taper
- Self-tapping thread
- Manufactured from grade 4 pure titanium with ultrapure homogeneous TiPure<sup>Plus</sup> surface
- Diameter: 3.25 · 3.75 · 4.1 · 4.5 · 5.5mm
- Lengths: 7 · 8.5 · 10 · 11.5 · 13mm



Consult instructions for use

SURGERY · S IMPLANTS WITH PM<sup>®</sup> DESIGN

Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Semados® implants</b> incl. cover screw and titanium insertion posts TiPure <sup>Plus</sup> surface Material: Titanium grade 4 (packaged sterile)	57500	■	3.25 L8.5	S	1
	57501	■	3.25 L10	S	1
	57502	■	3.25 L11.5	S	1
	57503	■	3.25 L13	S	1
	57601	■■	3.75 L8.5	S	1
	57602	■■	3.75 L10	S	1
	57603	■■	3.75 L11.5	S	1
	57604	■■	3.75 L13	S	1
	57840	■■■	4.1 L7	S	1
	57841	■■■	4.1 L8.5	S	1
	57842	■■■	4.1 L10	S	1
	57843	■■■	4.1 L11.5	S	1
	57844	■■■	4.1 L13	S	1
	57700	■■■■	4.5 L7	S	1
	57701	■■■■	4.5 L8.5	S	1
	57702	■■■■	4.5 L10	S	1
	57703	■■■■	4.5 L11.5	S	1
	57704	■■■■	4.5 L13	S	1
	57901	■■■■■	5.5 L8.5	S	1
	57902	■■■■■	5.5 L10	S	1
	57903	■■■■■	5.5 L11.5	S	1
	57904	■■■■■	5.5 L13	S	1
<b>BEGO SECURITY implants**<sup>4</sup></b> Implant warranty	83538				1

**Note:** BEGO Semados® S implants 3.25–4.5, template-guided preparation using the BEGO Guide System is an option.

**\*Please take into consideration the particular warranty conditions in the BEGO SECURITY implants product information. RFF 83528. May not be available in all countries.**

\*<sup>7</sup> Platform Switch design



## OVERVIEW

Cover screws	<b>40</b>
Healing abutments	<b>40</b>

SURGERY · COVER SCREWS/HEALING ABUTMENTS WITH PM<sup>®</sup> DESIGN

## Cover screws

Description	REF	Color code	Size	Compatibility	Units
<b>Implant cover screws</b>	55505	■		S 3.25	1
Material: Titanium grade 4 (packaged sterile)	55608	■		S/RI 3.75	1
Tool: Hexagon screwdriver 1.25mm	55615	■		S/RI 4.1	1
*2	55616	■		S/RI 4.5	1
	55908	■		S/RI 5.5	1



## **Healing abutments**

Description	REF	Color code	Size	Compatibility			Units
<b>Healing abutments</b> prefabricated gingival former Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25mm/slot screwdriver *2				<b>Healing abutment Ø 4.0</b>			
	55590	■ ■	L3	S/RI	3.25–3.75		1
	55591	■ ■	L5	S/RI	3.25–3.75		1
	55592	■ ■	L7	S/RI	3.25–3.75		1
				<b>Healing abutment Ø 4.5</b>			
	56300	■ ■ ■ ■ ■	L3	S/RI	3.25–4.5		1
	56301	■ ■ ■ ■ ■	L5	S/RI	3.25–4.5		1
	56302	■ ■ ■ ■ ■	L7	S/RI	3.25–4.5		1
				<b>Healing abutment Ø 5.0</b>			
	55593	■ ■ ■ ■ ■	L3	S/RI	3.25–4.5		1
	55594	■ ■ ■ ■ ■	L5	S/RI	3.25–4.5		1
	55595	■ ■ ■ ■ ■	L7	S/RI	3.25–4.5		1
				<b>Healing abutment Ø 6.0</b>			
	56303	■ ■ ■ ■ ■ ■	L3	S/RI	3.25–5.5		1
	56304	■ ■ ■ ■ ■ ■	L5	S/RI	3.25–5.5		1
	56305	■ ■ ■ ■ ■ ■	L7	S/RI	3.25–5.5		1
<b>Healing abutment, conical</b> prefabricated gingival former for bar constructions Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25mm/slot screwdriver *2				<b>Healing abutments Ø 6.0</b>			
	57324	■ ■	L5	S/RI	3.25–3.75		1
<b>Healing abutment,</b> <b>individual</b> customisable gingival former comprising: • healing abutment • prosthesis screw Hex 1.25mm Material: Polyetheretherketone (PEEK) Tool: Hexagon screwdriver 1.25mm *2	55953	■ ■ ■ ■ ■	Ø 7.0	S/SC/SCX/RS/RSX/RI	3.25–5.5		1



<sup>\*2</sup> For torque specifications, see page 114.

\*<sup>7</sup> Platform Match design



## OVERVIEW

BEGO Guide System S/SC/SCX implants  
BEGO Guide System RS/RSX implants

42

45

## BEGO Guide System S/SC/SCX implants

Surgical tray					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Guide Tray</b> incl. container, fully loaded	57399			S/SC/SCX 3.25–4.5	1
					
Master sleeves					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Guide master sleeves</b>	57395		Ø 4.2 (A)	S/SC/SCX/RS/RSX	10
	57397		Ø 4.7 (B)	S/SC/SCX/RS/RSX	10
					
Reduction sleeves					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Guide spoons</b>	57411		Ø 1.6 (A1)	S/SC/SCX	1
	57412		Ø 2.5 (A2)	S/SC/SCX	1
	57413		Ø 2.8 (A3)	S/SC/SCX 3.25	1
	57414		Ø 3.25 (A4)	S/SC/SCX 3.75	1
	57415		Ø 1.6 (B1)	S/SC/SCX	1
	57416		Ø 2.5 (B2)	S/SC/SCX	1
	57417		Ø 2.8 (B3)	S/SC/SCX 3.25	1
	57418		Ø 3.25 (B4)	S/SC/SCX 3.75	1
	57419		Ø 3.65 (B5)	S/SC/SCX 4.1	1
	57420		Ø 4.0 (B6)	S/SC/SCX 4.5	1
					
Tissue punches					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Guide tissue punches</b>	57421	□ ■ ■	Ø 4.2 (A)	S/SC/SCX/RS/RSX 3.0–3.75	1
	57422	■ ■	Ø 4.7 (B)	S/SC/SCX/RS/RSX 4.1–4.5	1
					

## BEGO Guide System S/SC/SCX implants

Preparation instruments							
Description	REF	Color code	Size	Compatibility	Units		
BEGO Guide centre drill	57459		Ø 4.2 (A)	S/SC/SCX/RS/RSX	3.0–3.75	1	
	57463		Ø 4.7 (B)	S/SC/SCX/RS/RSX	4.1–4.5	1	
BEGO Guide pilot drill	57423		Ø 1.6 L18 (X1)	S/SC/SCX	1		
	57424		Ø 1.6 L23.5 (Y1)	S/SC/SCX	1		
	57425		Ø 1.6 L29 (Z1)	S/SC/SCX	1		
BEGO Guide depth drill	57426		Ø 2.5 L18 (X2)	S/SC/SCX	1		
	57427		Ø 2.5 L23.5 (Y2)	S/SC/SCX	1		
	57428		Ø 2.5 L29 (Z2)	S/SC/SCX	1		
BEGO Guide depth drill	57429	■	Ø 2.8 L18 (X3)	S/SC/SCX	3.25	1	
	57430	■	Ø 2.8 L23.5 (Y3)	S/SC/SCX	3.25	1	
	57431	■	Ø 2.8 L29 (Z3)	S/SC/SCX	3.25	1	
BEGO Guide depth drill	57432	■	Ø 3.25 L18 (X4)	S/SC/SCX	3.75	1	
	57433	■	Ø 3.25 L23.5 (Y4)	S/SC/SCX	3.75	1	
	57434	■	Ø 3.25 L29 (Z4)	S/SC/SCX	3.75	1	
BEGO Guide depth drill	57435	■	Ø 3.65 L18 (X5)	S/SC/SCX	4.1	1	
	57436	■	Ø 3.65 L23.5 (Y5)	S/SC/SCX	4.1	1	
	57437	■	Ø 3.65 L29 (Z5)	S/SC/SCX	4.1	1	
BEGO Guide depth drill	57438	■	Ø 4.0 L18 (X6)	S/SC/SCX	4.5	1	
	57439	■	Ø 4.0 L23.5 (Y6)	S/SC/SCX	4.5	1	
	57441	■	Ø 4.0 L29 (Z6)	S/SC/SCX	4.5	1	
BEGO Guide countersink	57442	■	(3)	S/SC/SCX	3.25	1	
	57443	■	(4)	S/SC/SCX	3.75	1	
	57444	■	(5)	S/SC/SCX	4.1	1	
	57445	■	(6)	S/SC/SCX	4.5	1	

## BEGO Guide System S/SC/SCX implants

Preparation instruments					
Description	REF	Color code	Size	Compatibility	Units
BEGO Guide thread tap	57446	■	(3)	S/SC/SCX 3.25	1
	57447	■	(4)	S/SC/SCX 3.75	1
	57448	■	(5)	S/SC/SCX 4.1	1
	57449	■	(6)	S/SC/SCX 4.5	1



Connector					
Description	REF	Color code	Size	Compatibility	Units
BEGO Guide connector	57450		Ø 4.2 (AX)	S/SC/SCX	1
	57451		Ø 4.2 (AY)	S/SC/SCX	1
	57452		Ø 4.2 (AZ)	S/SC/SCX	1
	57453		Ø 4.7 (BX)	S/SC/SCX	1
	57454		Ø 4.7 (BY)	S/SC/SCX	1
	57455		Ø 4.7 (BZ)	S/SC/SCX	1
BEGO Guide depth stop ring connector	57456		Ø 4.2 (A)	S/SC/SCX/RS/RSX	1
	57457		Ø 4.7 (B)	S/SC/SCX/RS/RSX	1
BEGO Guide ratchet adapter for connector	57458			S/SC/SCX	1



Watch video "BEGO Guide Tray (S/SC/SCX)":



## BEGO Guide System RS/RSX implants

Surgical tray					
Description	REF	Color code	Size	Compatibility	Units
BEGO Guide tray incl. container, fully loaded	58071			RS/RSX 3.0–4.5	1
BEGO Guide tray (empty) empty tray, with container	58386			RS/RSX 3.0–4.5	1
Master sleeves					
Description	REF	Color code	Size	Compatibility	Units
BEGO Guide master sleeves	57395		Ø 4.2 (A)	S/SC/SCX/RS/RSX	10
	57397		Ø 4.7 (B)	S/SC/SCX/RS/RSX	10
Reduction sleeves					
Description	REF	Color code	Size	Compatibility	Units
BEGO Guide Sp	57686		Ø 2.0 (A1)	RS/RSX	1
	57687		Ø 2.5 (A2)	RS/RSX	1
	57688		Ø 2.8 (A3)	RS/RSX 3.0	1
	57689		Ø 3.4 (A4)	RS/RSX 3.75	1
	57690		Ø 2.0 (B1)	RS/RSX	1
	57691		Ø 2.5 (B2)	RS/RSX	1
	57692		Ø 2.8 (B3)	RS/RSX 3.0	1
	57693		Ø 3.4 (B4)	RS/RSX 3.75	1
	57694		Ø 3.8 (B5)	RS/RSX 4.1	1
	57695		Ø 4.1 (B6)	RS/RSX 4.5	1
Tissue punches					
Description	REF	Color code	Size	Compatibility	Units
BEGO Guide tissue punches	57421	□ ■ ■	Ø 4.2 (A)	S/SC/SCX/RS/RSX 3.0–3.75	1
	57422	■ ■	Ø 4.7 (B)	S/SC/SCX/RS/RSX 4.1–4.5	1



## BEGO Guide System RS/RSX implants

Preparation instruments							
Description	REF	Color code	Size	Compatibility	Units		
<b>BEGO Guide centre drill</b> Pilot drill	57459		Ø 4.2 (A)	S/SC/SCX/RS/RSX	3.0–3.75	1	
	57463		Ø 4.7 (B)	S/SC/SCX/RS/RSX	4.1–4.5	1	
<b>BEGO Guide PD</b> Pilot drill	57696		Ø 2.0 L18 (X1)	RS/RSX	1		
	57697		Ø 2.0 L23.5 (Y1)	RS/RSX	1		
	57698		Ø 2.0 L29 (Z1)	RS/RSX	1		
<b>BEGO Guide DD</b> Depth drill	57713		Ø 2.5 L18 (X2)	RS/RSX	1		
	57714		Ø 2.5 L23.5 (Y2)	RS/RSX	1		
	57715		Ø 2.5 L29 (Z2)	RS/RSX	1		
<b>BEGO Guide DD</b> Depth drill	57716	□	Ø 2.8 L18 (X3)	RS/RSX	3.0	1	
	57717	□	Ø 2.8 L23.5 (Y3)	RS/RSX	3.0	1	
	57723	□	Ø 2.8 L29 (Z3)	RS/RSX	3.0	1	
<b>BEGO Guide DD</b> Depth drill	57724	■	Ø 3.4 L18 (X4)	RS/RSX	3.75	1	
	57725	■	Ø 3.4 L23.5 (Y4)	RS/RSX	3.75	1	
	57726	■	Ø 3.4 L29 (Z4)	RS/RSX	3.75	1	
<b>BEGO Guide DD</b> Depth drill	57727	■	Ø 3.8 L18 (X5)	RS/RSX	4.1	1	
	57733	■	Ø 3.8 L23.5 (Y5)	RS/RSX	4.1	1	
	57734	■	Ø 3.8 L29 (Z5)	RS/RSX	4.1	1	
<b>BEGO Guide DD</b> Depth drill	57735	■	Ø 4.1 L18 (X6)	RS/RSX	4.5	1	
	57736	■	Ø 4.1 L23.5 (Y6)	RS/RSX	4.5	1	
	57737	■	Ø 4.1 L29 (Z6)	RS/RSX	4.5	1	
<b>BEGO Guide CS</b> Countersink	58051	□	(3)	RS/RSX	3.0	1	
	58052	■	(4)	RS/RSX	3.75	1	
	58053	■	(5)	RS/RSX	4.1	1	
	58054	■	(6)	RS/RSX	4.5	1	

## BEGO Guide System RS/RSX implants

Preparation instruments					
Description	REF	Color code	Size	Compatibility	Units
BEGO Guide ST Thread tap	58055	□	(3)	RS/RSX 3.0	1
	58056	■	(4)	RS/RSX 3.75	1
	58057	■	(5)	RS/RSX 4.1	1
	58058	■	(6)	RS/RSX 4.5	1

Connector					
Description	REF	Color code	Size	Compatibility	Units
BEGO Guide Conn with contra-angle connection	58059		Ø 4.2 (AX)	RS/RSX	1
	58060		Ø 4.2 (AY)	RS/RSX	1
	58061		Ø 4.2 (AZ)	RS/RSX	1
	58062		Ø 4.7 (BX)	RS/RSX	1
	58063		Ø 4.7 (BY)	RS/RSX	1
	58064		Ø 4.7 (BZ)	RS/RSX	1

BEGO Guide Conn with ratchet connection	58065		Ø 4.2 (AX)	RS/RSX	1
	58066		Ø 4.2 (AY)	RS/RSX	1
	58067		Ø 4.2 (AZ)	RS/RSX	1
	58068		Ø 4.7 (BX)	RS/RSX	1
	58069		Ø 4.7 (BY)	RS/RSX	1
	58070		Ø 4.7 (BZ)	RS/RSX	1

BEGO Guide depth stop ring connector	57456		Ø 4.2 (A)	S/SC/SCX/RS/RSX	1
	57457		Ø 4.7 (B)	S/SC/SCX/RS/RSX	1

Watch video "BEGO Guide Tray (RS/RSX)":



## BEGO Guide System – Guided pilot drill holes

Preparation instruments					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Guide – pilot drill</b> for guided surgical pilot drill holes	57400		Ø 2.0 L22		1
	57401		Ø 2.0 L30		1



Drill sleeves					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Guide DS</b> for guided surgical pilot drill holes	57130		Ø 2.0		10





## OVERVIEW

BEGO Semados® S/SC/SCX implants	50
BEGO Semados® RS/RSX implants	53
BEGO Semados® RI implants	56
Surgical instruments	58
Bone shapers/trepans	59

## BEGO Semados® S/SC/SCX implants

Surgical tray					
Description	REF	Color code	Size	Compatibility	Units
BEGO Semados® Tray <sup>Plus</sup> incl. container, excl. drill module Ø 5.5 (REF 57347)	57340			S/SC/SCX 3.25–5.5	1
BEGO Semados® Tray <sup>Plus</sup> (empty) empty tray, with container	58351			S/SC/SCX 3.25–5.5	1
Drill module					
Description	REF	Color code	Size	Compatibility	Units
Drill module comprising: • depth drill, short • countersink • thread tap with ratchet connection	57347	■		S/SC/SCX 5.5	1
Reduced basic surgical tray					
Description	REF	Color code	Size	Compatibility	Units
BEGO Semados® Starter/Compact Tray <sup>Plus</sup> incl. ratchet and container	58346			S/SC/SCX 3.75–4.5	1
BEGO Semados® Starter/Compact Tray <sup>Plus</sup> (empty) empty tray, with container	58347			S/SC/SCX 3.75–4.5	1
Preparation instruments					
Description	REF	Color code	Size	Compatibility	Units
Pilot marker	57308		Ø 1.6 L15	S/SC/SCX	1
	57309		Ø 1.6 L23	S/SC/SCX	1



**BEGO Semados® S/SC/SCX implants**

Preparation instruments					
Description	REF	Color code	Size	Compatibility	Units
Depth drill 2.5	57100		Ø 2.5 L15	S/SC/SCX	1
	57101		Ø 2.5 L20	S/SC/SCX	1
Depth drill	57102	■	Ø 2.8 L15	S/SC/SCX 3.25	1
	57104	■	Ø 3.25 L15	S/SC/SCX 3.75	1
	57106	■	Ø 3.65 L15	S/SC/SCX 4.1	1
	57108	■	Ø 4.0 L15	S/SC/SCX 4.5	1
	57110	■	Ø 4.7 L15	S/SC/SCX 5.5	1
Depth drill	57103	■	Ø 2.8 L20	S/SC/SCX 3.25	1
	57105	■	Ø 3.25 L20	S/SC/SCX 3.75	1
	57107	■	Ø 3.65 L20	S/SC/SCX 4.1	1
	57109	■	Ø 4.0 L20	S/SC/SCX 4.5	1
Countersink	57350	■		S/SC/SCX 3.25	1
	57351	■		S/SC/SCX 3.75	1
	57352	■		S/SC/SCX 4.1	1
	57353	■		S/SC/SCX 4.5	1
	57354	■		S/SC/SCX 5.5	1
Thread tap	57332	■		S/SC/SCX 3.25	1
	57333	■		S/SC/SCX 3.75	1
	57334	■		S/SC/SCX 4.1	1
	57335	■		S/SC/SCX 4.5	1
	57336	■		S/SC/SCX 5.5	1

**BEGO Semados® S/SC/SCX implants**

Drill stop sets					
Description	REF	Color code	Size	Compatibility	Quantity
<b>Drill stops</b>	55804			Depth drill 2.5 and S/SC/SCX 3.25–3.75	1 set
	55715			S/SC/SCX 4.1	1 set
	55810			S/SC/SCX 4.5	1 set
	55910			S/SC/SCX 5.5	1 set
<b>Drill stop Tray<sup>Plus</sup></b> incl. storage box, lid and all drill stops	57345			S/SC/SCX	1 unit
<b>Drill stop Tray<sup>Plus</sup> (empty)</b> empty storage box, with lid	58354			S/SC/SCX	1 unit

## BEGO Semados® RS/RSX implants

Surgical tray					
Description	REF	Color code	Size	Compatibility	Units
BEGO Semados® Tray <sup>Plus</sup> incl. container, excl. drill module Ø 5.5 (REF 57948)	57949			RS/RSX 3.0-5.5	1
BEGO Semados® Tray <sup>Plus</sup> (empty) empty tray, with container	58350			RS/RSX 3.0-5.5	1
Drill module					
Description	REF	Color code	Size	Compatibility	Units
Drill module comprising: • depth drill, short • DD D1 (depth drill) • countersink • thread tap	57948	■		RS/RSX 5.5	1
Reduced basic surgical tray					
Description	REF	Color code	Size	Compatibility	Units
BEGO Semados® Starter/Compact Tray <sup>Plus</sup> incl. ratchet and container	58348			RS/RSX 3.75-4.5	1
BEGO Semados® Starter/Compact Tray <sup>Plus</sup> (empty) empty tray, with container	58349			RS/RSX 3.75-4.5	1
Preparation instruments					
Description	REF	Color code	Size	Compatibility	Units
Pilot marker	57481		Ø 1.6 L15	RS/RSX	1
	57482		Ø 1.6 L23	RS/RSX	1
Depth drill 2.5	57926		Ø 2.5 L15	RS/RSX	1
	57927		Ø 2.5 L20	RS/RSX	1



**BEGO Semados® RS/RSX implants**

Preparation instruments					
Description	REF	Color code	Size	Compatibility	Units
Depth drill	57928	□	Ø 2.8 L15	RS/RSX	3.0
	57930	■	Ø 3.4 L15	RS/RSX	3.75
	57932	■	Ø 3.8 L15	RS/RSX	4.1
	57934	■	Ø 4.1 L15	RS/RSX	4.5
	57936	■	Ø 5.0 L15	RS/RSX	5.5
DD D1 (depth drill) In compact bone, particularly in the lower jaw, use depth drill DD D1 instead of the standard depth drill.	57484	□	Ø 2.9 L15	RS/RSX	3.0
	57485	■	Ø 3.6 L15	RS/RSX	3.75
	57486	■	Ø 4.0 L15	RS/RSX	4.1
	57487	■	Ø 4.3 L15	RS/RSX	4.5
	57488	■	Ø 5.3 L15	RS/RSX	5.5
Depth drill	57929	□	Ø 2.8 L20	RS/RSX	3.0
	57931	■	Ø 3.4 L20	RS/RSX	3.75
	57933	■	Ø 3.8 L20	RS/RSX	4.1
	57935	■	Ø 4.1 L20	RS/RSX	4.5
Countersink	57937	□		RS/RSX	3.0
	57938	■		RS/RSX	3.75
	57939	■		RS/RSX	4.1
	57940	■		RS/RSX	4.5
	57941	■		RS/RSX	5.5
Thread tap	57943	□		RS/RSX	3.0
	57944	■		RS/RSX	3.75
	57945	■		RS/RSX	4.1
	57946	■		RS/RSX	4.5
	57947	■		RS/RSX	5.5



## BEGO Semados® RS/RSX implants

Drill stop sets					
Description	REF	Color code	Size	Compatibility	Quantity
Drill stops	57476		Depth drill 2.5	RS/RSX	1 set
	57477	□		RS/RSX 3.0	1 set
	57478	■		RS/RSX 3.75	1 set
	57479	■■		RS/RSX 4.1–4.5	1 set
	57480	■■■		RS/RSX 5.5	1 set
Drill stop Tray <sup>Plus</sup> incl. storage box, lid and all drill stops	57483			RS/RSX	1 unit
Drill stop Tray <sup>Plus</sup> (empty) empty storage box, with lid	58356			RS/RSX	1 unit



## BEGO Semados® RI implants

Surgical tray					
Description	REF	Color code	Size	Compatibility	Units
<b>BEGO Semados® Tray<sup>Plus</sup></b> incl. container, excl. drill module Ø 5.5 (REF 57613)	57612			RI 3.75–5.5	1
<b>BEGO Semados® Tray<sup>Plus</sup></b> (empty) empty tray, with container	58352			RI 3.75–5.5	1

Drill module					
Description	REF	Color code	Size	Compatibility	Units
<b>Drill module</b> comprising: <ul style="list-style-type: none"><li>• depth drill</li><li>• countersink</li><li>• threadformer</li><li>• screw tap</li></ul>	57613	■		RI 5.5	1

Preparation instruments					
Description	REF	Color code	Size	Compatibility	Units
<b>Pilot marker</b>	57581		Ø 2.5 L16	RI	1
	57582		Ø 2.5 L25	RI	1
<b>Depth drill 3.2</b>	57583		Ø 3.2 L15	RI	1
	57584		Ø 3.2 L20	RI	1

**BEGO Semados® RI implants****Preparation instruments**

Description	REF	Color code	Size	Compatibility	Units	
Depth drill	57585	■	Ø 3.52 L15	RI 3.75	1	
	57587	■	Ø 3.93 L15	RI 4.1	1	
	57589	■	Ø 4.32 L15	RI 4.5	1	
	57591	■	Ø 5.28 L15	RI 5.5	1	
Depth drill	57586	■	Ø 3.52 L20	RI 3.75	1	
	57588	■	Ø 3.93 L20	RI 4.1	1	
	57590	■	Ø 4.32 L20	RI 4.5	1	
Countersink	57592	■		RI 3.75	1	
	57593	■		RI 4.1	1	
	57594	■		RI 4.5	1	
	57595	■		RI 5.5	1	
Threadformer	55766	■		RI 3.25	1	
	57615	■		RI 3.75	1	
	57616	■		RI 4.1	1	
	57617	■		RI 4.5	1	
	57618	■		RI 5.5	1	
Thread tap	57619	■		RI 3.75	1	
	57620	■		RI 4.1	1	
	57621	■		RI 4.5	1	
	57622	■		RI 5.5	1	

## Surgical instruments

Surgical instruments					
Description	REF	Color code	Size	Compatibility	Units
<b>Drill extension, one-part without internal cooling</b>	57265			Extension of 15.8mm	1
					
<b>Insert tool for implants with ratchet connection</b>	55831		L6		1
	55830		L12.5		1
					
<b>Insert tool for implants with contra-angle connection</b>	56990		L21.5		1
	55832		L24		1
					
<b>IDC (adjustment instrument) for making final corrections to the position of the inserted implant after removal of the insertion post</b>	56749	□		RS/RSX 3.0	1
	56748			S/SC/SCX/RS/RSX/RI 3.25–5.5	1
					
<b>Guiding wrench spanner and guide pin for tools with ratchet connection</b>	53897				1
					
<b>Paralleling post</b>	55863			S/SC/SCX	2
	57956			RS/RSX	2
	57598			RI	1
					

\*¹ Version of the BEGO Semados® RI implants, with Platform Switch design

## Surgical instruments

Surgical instruments					
Description	REF	Color code	Size	Compatibility	Units
Depth gauge	53872			S/SC/SCX	1
	55746			RI	1
	57955			RS/RSX	1
					
Ratchet/ torque wrench for torques 10–50Ncm	55799				1
					
BEGO Semados® ratchet adapter with ratchet connection for universal use of the ratchet (ratchet grips the adapter head / adapter shaft holds the dental shaft as described in EN ISO 1797-1)	55599				1
					

## Bone shapers/trepans

Bone shapers					
Description	REF	Color code	Size	Compatibility	Units
PS BP	58445	□		SC/SCX/RS/RSX/RI*3.0	1
	58446	■■		SC/SCX/RS/RSX/RI*3.25–3.75	1
	58447	■		SC/SCX/RS/RSX/RI*4.1	1
	58448	■		SC/SCX/RS/RSX/RI*4.5	1
	58449	■		SC/SCX/RS/RSX/RI*5.5	1
					

## Trepan drill

Trepan drill					
Description	REF	Color code	Size	Compatibility	Units
Trepan drill	55817		Ø 4.2 external/Ø 3.7 internal	L20	1
	55815		Ø 5.0 external/Ø 4.1 internal	L20	1
	56991		Ø 5.0 external/Ø 4.3 internal	L20	1
	55816		Ø 6.0 external/Ø 5.1 internal	L20	1
					





## OVERVIEW

Instruments	62
CAD/CAM Implant Prosthetics BEGO Medical	63
Prosthetics SC/SCX/RS/RSX/RI* <sup>1</sup> implants (Platform Switch design)	71
Prosthetics S implants (Platform Match design)	91

## PROSTHETICS · INSTRUMENTS

### Prosthetic tray

Description	REF	Color code	Size	Compatibility	Units	
<b>Prosthetic kit</b> with ratchet/torque wrench, hexagon screwdriver 1.25mm short/long, slot screwdriver long, insert tool for ball attachment, insert tool 3Locator®, ratchet adapter, incl. storage box and lid	55826				1	
<b>Prosthetic kit (empty)</b> empty storage box, with lid	58357				1	

### Prosthetic instruments

Description	REF	Color code	Size	Compatibility	Units	
<b>Hexagon screwdriver 1.25mm</b> with conical ratchet connection for implant cover screws, healing abutments, impression posts, insertion posts and prosthesis screws	57266		L5		1	
	53949		L10		1	
	53948		L17		1	
<b>Hexagon screwdriver 1.25mm contra-angle</b> conical for implant cover screws, healing abutments, impression posts, insertion posts and Prosthesis screws	55563		L25		1	
	55564		L31		1	
<b>Slot screwdriver</b> with ratchet connection For healing abutments and impression posts	53952		L14		1	
<b>Ratchet/torque wrench</b> for torques 10–50Ncm	55799				1	
<b>BEGO Semados® ratchet adapter</b> with ratchet connection for universal use of the ratchet (ratchet grips the adapter head / adapter shaft holds the dental shaft as described in EN ISO 1797-1)	55599				1	

**Note:** Manufacturer notes about trade names, see page 111.



## OVERVIEW

Interface overview	64
Individual healing abutments	65
Individual abutments	65
Occlusal screw-retained bridge restorations	67
Bar constructions	68

Interface overview								
Implant diameter	Platform	Color code	CADAbut Full	CADAbut Duo with anti-rotation protection	CADAbut Duo without anti-rotation protection	CADBase implant level	CADBase abutment level	
			 	     	   	 		
<b>BEGO Implant Systems – Semados® SC/SCX/RS/RSX/RI implants – Platform Switch design</b>								
RS/RSX 3.0	3.0	□						
SC/SCX 3.25	3.67	■						
SC/SCX/RS/RSX/RI 3.75	3.67	■	✓					
SC/SCX/RS/RSX/RI 4.1	4.1	■		✓				
SC/SCX/RS/RSX/RI 4.5	4.5	■				✓	✓	✓
SC/SCX/RS/RSX/RI 5.5	5.5	■						
<b>BEGO Implant Systems – Semados® S implants – Platform Match design</b>								
3.25	3.67	■						
3.75	3.67	■						
4.1	4.1	■	✓			✓	✓	✓
4.5	4.5	■			✓			
5.5	5.5	■						
<b>BEGO Implant Systems – Semados® Multiplus</b>								
3.25; 3.75; 4.1; 4.5; 5.5	Abutment level							✓

## Individual healing abutments – patient-specific soft tissue management for outstanding aesthetics

<b>BEGO CADAbut Full – one-part individual healing abutments incl. prosthesis screw</b>	
Description	Units
BEGO titanium grade 5 only for temporary use	1
	
<b>BEGO CADAbut Duo – two-part individual healing abutments (plus titanium adhesive abutment)</b>	
Description	Units
BEGO PMMA Multicolor available in 3 shades (M01, M02, M03), only for temporary use	1
	

## Individual abutments – one- and two-part abutments

<b>BEGO CADAbut Full – one-part individual abutments incl. prosthesis screw</b>	
Description	Units
Wirobond® MI+	1
	
BEGO titanium grade 5	1
	
Extras Fully anatomical shape	1
	

<b>BEGO CADAbut Duo – two-part individual healing abutments (plus titanium adhesive abutment)</b>		
Description	Compatibility	Units
<b>BEGO Zirkon LT</b> available in 5 shades (LT01–LT05)		1
		
<b>KATANA<sup>®</sup> Zirconia STML</b> available in 13 VITA <sup>®</sup> classical shades.		1
		
<b>IPS e.max<sup>®</sup> CAD</b> Delivered in blue pre-crystallized state. LT can be supplied in the 16 VITA <sup>®</sup> classical shades. MO can be supplied in five opaque shades.	SC/SCX/RS/RSX/RI <sup>†</sup>	1
		
<b>CAD/Cast<sup>®</sup> alloys</b> Selected BEGO precious metal alloys at the currently valid daily price; request the current prices. (Tel. +49 421 20 28-251)		1
		
<b>Wirobond<sup>®</sup> C+</b>		1
		
<b>BEGO PMMA Multicolor</b> available in 3 shades (M01, M02, M03), only for temporary use		1
		

<sup>†</sup> Only for BEGO Semados<sup>®</sup> implants with Platform Switch design.<sup>®</sup>This symbol is a commercial name/registered trademark of a company that does not belong to the BEGO Group.

## Occlusal screw-retained one- and two-part bridge restorations

### BEGO CADBase implant level/abutment level – one-part individual bridge constructions incl. prosthesis screw

Description	Product description	Units	
<b>BEGO titanium grade 5</b>	Occlusal screw-retained bridge/framework	2–4	
	Occlusal screw-retained bridge/framework	5–7	
	Occlusal screw-retained bridge/framework	≥ 8	
	Angled screw channel 0°–20°		
	Pontic/bridge member		
<b>Wirobond® M+</b>	Occlusal screw-retained bridge/framework	2–4	
	Occlusal screw-retained bridge/framework	5–7	
	Occlusal screw-retained bridge/framework	≥ 8	
	Angled screw channel 0°–20°		
	Pontic/bridge member		

### DYNAMIC ABUTMENT®

Description	REF	Units	
Screwdriver L24 for prosthesis screw angled screw channels	549539	1	

### BEGO CADAbut Duo without anti-rotation protection – two-part individual bridge constructions (plus titanium adhesive abutment)

Description	Product description	Units	
<b>BEGO Zirkon LT</b> Bridge constructions for partial and full veneers with up to 16 units and up to two bridge members, available in five shades (LT01–LT05)	Occlusal screw-retained bridge/framework	up to 16	
	Pontic/bridge member	up to 2	
<b>KATANA®<sup>6</sup> Zirconia STML</b> up to three units, available in 13 VITA <sup>®</sup> classical shades	Occlusal screw-retained bridge/framework	up to 3	
	Pontic/bridge member	up to 1	
<b>BEGO PMMA Multicolor</b> Only for temporary bridge restorations With up to 16 units and one pontic, available in three shades (M01, M02, M03).	Occlusal screw-retained bridge/framework	up to 16	
	Pontic/bridge member	up to 1	
<b>Wirobond® C+</b> Bridge constructions for partial and full veneers with up to 16 units and up to four bridge members	Occlusal screw-retained bridge/framework	up to 4	
	Pontic/bridge member	≥ 4	
	Pontic/bridge member	> 4	
Fully anatomical bridge construction with up to 16 units and up to four bridge members	Occlusal screw-retained bridge/framework	up to 4	
	Pontic/bridge member	≥ 4	
	Pontic/bridge member	> 4	

## Bar constructions – milled bars and bar bases made from titanium or cobalt-chromium

BEGO CADBase (bar bases incl. prosthesis screws)	
Description	Number of implant units
BEGO titanium grade 5	2–4
	5–7
	≥ 8
Wirobond® Mi+	2–4
	5–7
	≥ 8



BEGO CADBar	
Description	Units
BEGO titanium grade 5	1
Wirobond® Mi+	1



Bar joint attachments	
Description	Cross-section
Round bar 1.8mm	
Horix® <sup>6</sup> bar 1.8mm	
Dolder® <sup>6</sup> bar joint attachment 2.3mm	
Dolder® <sup>6</sup> bar joint attachment 3.0mm	

**Indication:** Implant/mucosa-supported removable prosthesis on at least two implants (without extensions)

**Note:** Bridge constructions not available for BEGO Semados® RS/RSX implants Ø3.0 and Mini implants!

<sup>6</sup>This symbol is a commercial name/registered trademark of a company that does not belong to the BEGO Group.

**Bar attachments****Description****Cross-section**

Dolder<sup>\*6</sup> bar attachments  
3.0mm



Individual bar shapes/  
bar attachments



**Indication:** Implant-supported removable prosthesis on at least four implants (with extensions)

**Additional retention elements****Description****Units****Bar attachments****available for:**

- Ancora<sup>\*6</sup> / Preci-Vertix<sup>\*6</sup> 1.8mm
- Preci-Vertix<sup>\*6</sup> Crown
- Preci-Vertix<sup>\*6</sup> Bar

1

**Thread drills for retention  
elements,****available for:**

- Zest Anchors<sup>\*6</sup>
- CEKA<sup>\*6</sup> attachment M2
- CEKA<sup>\*6</sup> attachment M3
- CEKA<sup>\*6</sup> ball anchor M2

1

**Drill elements**

1.9–3.0mm

1

**Bar element**Preci-Horix<sup>\*6</sup> 1.8mm

1

**Retention elements****Description**

Dolder<sup>\*6</sup> bar female parts  
**palladium alloy**  
Resilience bar attachments,  
female parts with retention  
for polymer



available from  
Ceka-Vertrieb Deutschland,  
Akazienstraße 7A, 30169 Hanover,  
Germany  
Tel. +49 511 8070041,  
[www.cka-vertrieb.de](http://www.cka-vertrieb.de)

**Ancora female parts (Preci-Vertix rider/Preci-Horix<sup>\*6</sup> rider)**

Description	REF	Size	Units
<b>Ancora</b> Universal rider rigid	52593	Ø 1.8mm	1
Also available from BEGO Bremer Goldschlägerei Wilh. Herbst GmbH & Co. KG, Wilhelm-Herbst-Str. 1, 28359 Bremen, Germany, Tel. +49 421 2028-0, Fax +49 421 2028-100, email: info@bego.com, www.bego.com			

**Bar secondary structure**

Description	Units
<b>Wirobond® C+</b> including pin, hole, and / or bead retentions	1
<b>Hybrid with Wirobond® C+</b> including pin, hole and / or bead retentions	i



For questions about individually fabricated CAD/CAM implant prosthetics from BEGO Medical GmbH (procedure or conditions), please contact:

BEGO Medical GmbH  
Wilhelm-Herbst-Str. 1 · 28359 Bremen,  
Germany

Tel. +49 421 2028-0 · Fax +49 421 2028-174  
email info@bego-medical.de · www.bego.com

**Note:** Bridge constructions not available for BEGO Semados® RS/RX implants Ø3.0 and Mini implants!

\*<sup>1</sup> Version of the BEGO Semados® RI implant, with Platform Switch design

\*<sup>5</sup> Platform Switch design

\*<sup>6</sup> This symbol is a commercial name/registered trademark of a company that does not belong to the BEGO Group.



## OVERVIEW

CAD/CAM restoration	<b>72</b>
Impression taking and model fabrication	<b>75</b>
Crown restoration Ø 3.0	<b>76</b>
Crown and bridge restoration	<b>77</b>
Multi <sup>Plus</sup> restoration	<b>82</b>
Hybrid restoration	<b>86</b>
Screws	<b>89</b>

**Note:** The entire Platform Switch prosthetics range is **not** compatible with the previous S/RI implants (with the Platform Match design)! For these implants, please only use the structures/components listed from page 91 onward.

## CAD/CAM restoration Ø 3.0

CAD positioner					
Description	REF	Color code	Size	Compatibility	Units
<b>PS CADP</b> comprising: • PS CAD positioner • PScrew Material: Titanium grade 4 Tool: Hexagon screwdriver 1.25mm *2	58250	□		RS/RSX 3.0	1



Adhesive abutment					
Description	REF	Color code	Size	Compatibility	Units
<b>PS TiB</b> comprising: • PS adhesive abutment • PScrew • TScrew Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57781	□		RS/RSX 3.0	1



**Note:** When using the \*<sup>6</sup>Cerec® system, a \*<sup>6</sup>Cerec/\*<sup>6</sup>InLab scanbody for \*<sup>6</sup>Bluecam (36 units) REF 6431303 or a scanbody for \*<sup>6</sup>Omnicam (36 units) REF 6431329 (Sirona Dental Systems GmbH, Bensheim, Germany) is required.

\*<sup>1</sup> Version of the BEGO Semados® RI implants, with Platform Switch design

\*<sup>2</sup> For torque specifications, see page 114

\*<sup>5</sup> Platform Switch design

**CAD/CAM restoration Ø 3.25–5.5**

CAD positioner					
Description	REF	Color code	Size	Compatibility	Units
<b>PS CADP</b> comprising: <ul style="list-style-type: none"><li>• PS CAD positioner</li><li>• prosthesis screw Hex 1.25mm</li></ul> Material: Titanium grade 4 Tool: Hexagon screwdriver 1.25mm *2	58251	■■		SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	58252	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58253	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	58254	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1



Adhesive abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>PS TiB</b> comprising: <ul style="list-style-type: none"><li>• PS adhesive abutment Hex</li><li>• prosthesis screw Sub-Tec<sup>Plus</sup></li><li>• technician screw Sub-Tec<sup>Plus</sup></li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57823	■■	GH 0	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	58370	■■	GH 1.5	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	57824	■	GH 0	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58371	■	GH 1.5	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	57825	■	GH 0	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	58372	■	GH 1.5	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	57826	■	GH 0	SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1
	58373	■	GH 1.5	SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1



Scansupports					
Description	REF	Color code	Size	Compatibility	Units
<b>CAD SP</b> comprising: <ul style="list-style-type: none"><li>• scansupport</li><li>• prosthesis screw Sub-Tec<sup>Plus</sup></li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	58191	■■		S/SC/SCX/RS/RSX/RI 3.25–3.75	1
	58192	■		S/SC/SCX/RS/RSX/RI 4.1	1
	58193	■		S/SC/SCX/RS/RSX/RI 4.5	1
	58194	■		S/SC/SCX/RS/RSX/RI 5.5	1



Options for downloading adhesive geometries for decentralized fabrication are available online at [www.bego.com](http://www.bego.com)

## CAD/CAM restoration Ø 3.25–5.5

Adhesive abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>PS TiB NH</b> comprising: <ul style="list-style-type: none"><li>• PS adhesive abutment no Hex</li><li>• prosthesis screw Sub-Tec<sup>Plus</sup></li><li>• technician screw Sub-Tec<sup>Plus</sup></li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57827		GH 0	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	58374		GH 1.5	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	57828		GH 0	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58375		GH 1.5	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	57829		GH 0	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	58376		GH 1.5	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	57830		GH 0	SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1
	58377		GH 1.5	SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1



Milling blank					
Description	REF	Color code	Size	Compatibility	Units
<b>PS PMB</b> comprising: <ul style="list-style-type: none"><li>• milling blank</li><li>• prosthesis screw Sub-Tec<sup>Plus</sup></li><li>• technician screw Sub-Tec<sup>Plus</sup></li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	58326		Ø 11.5	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–5.5	1
	58226		Ø 16	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–5.5	1



Ti-Form milling blank					
Description	REF	Color code	Size	Compatibility	Units
<b>PS PMB</b> comprising: <ul style="list-style-type: none"><li>• milling blank Ti-Form</li><li>• prosthesis screw Sub-Tec<sup>Plus</sup></li><li>• technician screw Sub-Tec<sup>Plus</sup></li><li>• AmannGirrbach Intellicode</li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	58221			SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–5.5	1



ceramill® CAD/CAM

**Note:** Manufacturer notes about trade names, see page 111.

**Note:** For the PS PMB (milling blank) a \*<sup>6</sup>PreFace abutment holder for the corresponding milling system is required. This must be ordered directly from the machine manufacturer. Please note the manufacturer's information regarding this!

**Note:** PS PMB (Ti-Form milling blank), Original System Partner from ceramill CAD/CAM

\*<sup>1</sup> Version of the BEGO Semados® RI implants, with Platform Switch design

\*<sup>2</sup> For torque specifications, see page 114

\*<sup>5</sup> Platform Switch design

## Impression taking and model fabrication Ø 3.0–5.5

Impression sets					
Description	REF	Color code	Size	Compatibility	Units
<b>PS CTI</b> Impression taking on implant with closed tray comprising: <ul style="list-style-type: none"><li>• impression post cap</li><li>• PS impression post</li><li>• titanium screw</li></ul> Tool: Hexagon screwdriver 1.25mm <small>*2</small>	57773	□		RS/RSX 3.0	1
	58316	■		SC/SCX 3.25	1
	57799	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 3.75	1
	57800	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	57801	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	57802	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1
<b>PS OTI</b> Impression taking on implant with open tray comprising: <ul style="list-style-type: none"><li>• PS impression post</li><li>• titanium screw short/long</li></ul> Tool: Hexagon screwdriver 1.25mm <small>*2</small>	57774	□		RS/RSX 3.0	1
	58317	■		SC/SCX 3.25	1
	57803	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 3.75	1
	57804	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	57805	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	57806	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1



Implant analogs					
Description	REF	Color code	Size	Compatibility	Units
<b>PS IMPA</b>	57796	□		RS/RSX 3.0	1
	58315	■		SC/SCX 3.25	1
	57819	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 3.75	1
	57820	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	57821	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	57822	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1



<sup>4</sup> DIM-Analogs®					
Description	REF	Color code	Size	Compatibility	Units
<b>BPS 5.DIM</b>	549320	□		RS/RSX 3.0	1
	549321	■■		SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	549322	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	549323	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	549324	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1



## Crown restoration Ø 3.0

Provisional					
Description	REF	Color code	Size	Compatibility	Units
<b>PS ITA</b> Material: Titanium alloy Tool: Insert tool for implants *2	57778	<input type="checkbox"/>		RS/RSX 3.0	1



Solid abutments, titanium					
Description	REF	Color code	Size	Compatibility	Units
<b>PS TiAA</b> angle over plane (type P) or edge (type E) comprising: <ul style="list-style-type: none"><li>• PS titanium abutment</li><li>• PScrew</li><li>• TScrew</li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57797	<input type="checkbox"/>	15° P GH 2.5–4	RS/RSX 3.0	1
	57798	<input type="checkbox"/>	15° E GH 2.5–4	RS/RSX 3.0	1
<b>PS TiA</b> comprising: <ul style="list-style-type: none"><li>• PS titanium abutment</li><li>• PScrew</li><li>• TScrew</li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57776	<input type="checkbox"/>	GH 2.5–4	RS/RSX 3.0	1



Angulated abutment, type P	Angulated abutment, type E
Type P = angle over plane	Type E = angle over edge



**Note:** Manufacturer notes about trade names, see page 111.

\*1 Version of the BEGO Semados® RI implants, with Platform Switch design

\*2 For torque specifications, see page 114

\*5 Platform Switch design

## Crown and bridge restoration Ø 3.25–5.5

Temporary abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>PS PPA</b> Solid abutment, plastic for provisional restorations comprising: • PS plastic abutment • prosthesis screw Hex 1.25mm • technician screw Material: Polyetheretherketone (PEEK) Tool: Hexagon screwdriver 1.25mm *2	58072	■■		SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	58073	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58074	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	58075	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1
<b>PS TPA</b> comprising: • PS plastic abutment • prosthesis screw Hex 1.25mm • technician screw Material: Polyetheretherketone (PEEK) Tool: Hexagon screwdriver 1.25mm *2	58146	■■		SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	58147	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58148	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
<b>PS TTiA</b> comprising: • provisional PS titanium abutment • prosthesis screw Sub-Tec <sup>Plus</sup> • technician screw Sub-Tec <sup>Plus</sup> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57854	■■		SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	57855	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	57856	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	57857	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1
<b>PS TTiA NH</b> comprising: • provisional PS titanium abutment no Hex • prosthesis screw Sub-Tec <sup>Plus</sup> • technician screw Sub-Tec <sup>Plus</sup> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57858	■■		SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	57859	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	57860	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	57861	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1
<b>PS ITA</b> Material: Titanium alloy Tool: Insert tool Implants *2	58076	■■		SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	58077	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58078	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1



## Crown and bridge restoration Ø 3.25–5.5

Solid abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>PS TiA</b> comprising: <ul style="list-style-type: none"><li>• PS titanium abutment, conical</li><li>• prosthesis screw Sub-Tec<sup>Plus</sup></li><li>• technician screw Sub-Tec<sup>Plus</sup></li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm * <sup>2</sup>	58088			SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	58089			SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58090			SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	58091			SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1



Solid abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>PS TiA</b> comprising: <ul style="list-style-type: none"><li>• PS titanium abutment</li><li>• prosthesis screw Sub-Tec<sup>Plus</sup></li><li>• technician screw Sub-Tec<sup>Plus</sup></li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm * <sup>2</sup>	57846		GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	57847		GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	57848		GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	57849		GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	57850		GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	57851		GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	57852		GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1
	57853		GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1



Selection set					
Description	REF	Color code	Size	Compatibility	Units
<b>PS AS</b> For selecting the correct abutment with corresponding gingival height and angle, comprising: <ul style="list-style-type: none"><li>• 20 parts + forceps</li></ul>	58247		0°/15°/20°	SC/SCX/RS/RSX/RI* <sup>1</sup>	1



Angulated abutment, type P		Angulated abutment, type E	
Type P = angle over plane		Type E = angle over edge	

\*<sup>1</sup> Version of the BEGO Semados® RI implants, with Platform Switch design

\*<sup>2</sup> For torque specifications, see page 114

\*<sup>3</sup> Alloy recommendation: Bio PontoStar® XL (BEGO, REF 61140)/Bio PontoStar® (BEGO, REF 61104)

\*<sup>5</sup> Platform Switch design

## Crown and bridge restoration Ø 3.25–5.5

### Solid abutments

Description	REF	Color code	Size	Compatibility	Units
<b>PS TiAA</b> angle over plane (type P) or edge (type E) comprising: <ul style="list-style-type: none"><li>• PS titanium abutment</li><li>• prosthesis screw Sub-Tec<sup>Plus</sup></li><li>• technician screw Sub-Tec<sup>Plus</sup></li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57889	■■	15° P GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	3.25–3.75
	57890	■■	15° P GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	3.25–3.75
	57891	■■	15° E GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	3.25–3.75
	57892	■■	15° E GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	3.25–3.75
	57893	■	15° P GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.1
	57894	■	15° P GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.1
	57895	■	15° E GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.1
	57896	■	15° E GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.1
	57897	■	15° P GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.5
	57898	■	15° P GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.5
	57899	■	15° E GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.5
	57900	■	15° E GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.5
	57905	■■	15° P GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	5.5
	57906	■■	15° P GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	5.5
	57907	■■	15° E GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	5.5
	57908	■■	15° E GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	5.5



### Solid abutments

Description	REF	Color code	Size	Compatibility	Units
<b>PS TiAA</b> angle over plane (type P) or edge (type E) comprising: <ul style="list-style-type: none"><li>• PS titanium abutment</li><li>• prosthesis screw Sub-Tec<sup>Plus</sup></li><li>• technician screw Sub-Tec<sup>Plus</sup></li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57909	■■	20° P GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	3.25–3.75
	57910	■■	20° P GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	3.25–3.75
	57911	■■	20° E GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	3.25–3.75
	57912	■■	20° E GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	3.25–3.75
	57913	■	20° P GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.1
	57914	■	20° P GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.1
	57915	■	20° E GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.1
	57916	■	20° E GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.1
	57917	■	20° P GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.5
	57918	■	20° P GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.5
	57919	■	20° E GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.5
	57920	■	20° E GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.5
	57921	■■	20° P GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	5.5
	57922	■■	20° P GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	5.5
	57923	■■	20° E GH 1–2	SC/SCX/RS/RSX/RI* <sup>1</sup>	5.5
	57924	■■	20° E GH 2.5–4	SC/SCX/RS/RSX/RI* <sup>1</sup>	5.5



Phase out by  
31.12.2021

## Crown and bridge restoration Ø 3.25–5.5

Universal abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>PS UNI</b> comprising: <ul style="list-style-type: none"><li>• PS universal base Hex</li><li>• wax-up sleeve Universal</li><li>• PS UNI PScrew</li><li>• PS UNI TScrew (black)</li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm * <sup>2</sup>	57831			SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	57832			SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	57833			SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	57834			SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1
<b>PS UNI NH</b> comprising: <ul style="list-style-type: none"><li>• PS universal base no Hex</li><li>• wax-up sleeve Universal</li><li>• PS UNI PScrew</li><li>• PS UNI TScrew (black)</li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm * <sup>2</sup>	57835			SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	57836			SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	57837			SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	57838			SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1
<b>Internal reamer Universal</b> For re-working the internal form fit	55536			S/SC/SCX/RS/RSX/RI 3.25–5.5	1
<b>External reamer Universal</b> For re-working the external form fit	55537			S/SC/SCX/RS/RSX/RI 3.25–5.5	1

Watch the video "BEGO Semados® Universal Abutment":



Watch the video "BEGO Semados® Universal Abutment no Hex":



\*<sup>1</sup> Version of the BEGO Semados® RI implants, with Platform Switch design

\*<sup>2</sup> For torque specifications, see page 114

\*<sup>3</sup> Alloy recommendation: Bio PontoStar® XL (BEGO, REF 61140)/Bio PontoStar® (BEGO, REF 61104)

\*<sup>5</sup> Platform Switch design

## Crown and bridge restoration Ø 3.25–5.5

### Gold cast-on abutments

Description	REF	Color code	Size	Compatibility	Units	
<b>PS GCO</b> comprising: <ul style="list-style-type: none"><li>• PS cast-on abutment</li><li>• wax-up sleeve for gold cast-on</li><li>• prosthesis screw Hex 1.25mm</li><li>• technician screw</li></ul> Material: Gold /platinum alloy Tool: Hexagon screwdriver 1.25mm *2 *3	58092	■■		SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1	
	58093	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1	
	58094	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1	
<b>PS GCO NH</b> comprising: <ul style="list-style-type: none"><li>• PS cast-on abutment no Hex</li><li>• wax-up sleeve for gold cast-on</li><li>• prosthesis screw Hex 1.25mm</li><li>• technician screw</li></ul> Material: Gold /platinum alloy Tool: Hexagon screwdriver 1.25mm *2 *3	58096	■■		SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1	
	58097	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1	
	58098	■		SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1	
	58099	■■		SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1	
<b>Internal reamer for gold cast-on abutment</b> For re-working the internal form fit (a technician screwdriver is recommended as the hold)	53735	■■■■■		S/SC/SCX/RS/RSX/RI 3.25–5.5	1	

## MultiPlus restoration

Auxiliary parts					
Description	REF	Color code	Size	Compatibility	Units
MultiPlus insertion splint To determine the planned angle	57532			MultiPlus System	1
MultiPlus alignment aids For aligning the implant hex	57530	20°		MultiPlus System	1
	57531	30°		MultiPlus System	1

Abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>PS MultiPlus</b> comprising: • PS abutment 0° • MultiPlus positioning aid 0° Material: Titanium alloy (packaged sterile) Tool: Insertion instrument MultiPlus abutment 0° *2	58100	■■	0° GH 1	SC/SCX/RS/RSX/RI* <sup>1</sup>	3.25–3.75
	58196*	■■	0° GH 2	SC/SCX/RS/RSX/RI	3.25–3.75
	58101	■■	0° GH 3	SC/SCX/RS/RSX/RI* <sup>1</sup>	3.25–3.75
	58216*	■■	0° GH 4	SC/SCX/RS/RSX/RI	3.25–3.75
	58102	■	0° GH 1	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.1
	58197*	■	0° GH 2	SC/SCX/RS/RSX/RI	4.1
	58103	■	0° GH 3	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.1
	58217*	■	0° GH 4	SC/SCX/RS/RSX/RI	4.1
	58104	■	0° GH 1	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.5
	58198*	■	0° GH 2	SC/SCX/RS/RSX/RI	4.5
	58105	■	0° GH 3	SC/SCX/RS/RSX/RI* <sup>1</sup>	4.5
	58218*	■	0° GH 4	SC/SCX/RS/RSX/RI	4.5
Insertion instrument MultiPlus abutment 0° with ratchet connection	57533			MultiPlus System	1
Insertion instrument MultiPlus abutment 0° with contra-angle connection	58199			MultiPlus System	1

Watch the video “BEGO Semados® MultiPlus System”:



\* Planned availability from November 2021

\*<sup>1</sup> Version of the BEGO Semados® RI implants with platform switch design

\*<sup>2</sup> For torque specifications, see page 114

\*<sup>5</sup> Platform Switch design

## MultiPlus restoration

Abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>PS MultiPlus</b> comprising: • PS MultiPlus abutment 20° • MultiPlus positioning aid 20° • prosthesis screw MultiPlus Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25mm *2	58108	■■	20° GH 2.3–0.6	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	58109	■■	20° GH 4.0–2.3	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	58110	■	20° GH 2.3–0.6	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58111	■	20° GH 4.0–2.3	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58112	■	20° GH 2.3–0.6	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	58113	■	20° GH 4.0–2.3	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
<b>PS MultiPlus</b> comprising: • PS MultiPlus abutment 30° • MultiPlus positioning aid 30° • prosthesis screw MultiPlus Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25mm *2	58116	■■	30° GH 4.0–1.5	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	58117	■	30° GH 4.0–1.5	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58118	■	30° GH 4.0–1.5	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
Healing posts					
Description	REF	Color code	Size	Compatibility	Units
<b>MultiPlus healing post</b> prefabricated gingival former Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25mm	57520		L5	MultiPlus System	1
<b>MultiPlus healing post</b> <b>Mushroom</b> prefabricated gingival former Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25mm	57521		L5	MultiPlus System	1



## MultiPlus restoration

Impression sets					
Description	REF	Color code	Size	Compatibility	Units
<b>MultiPlus closed-tray impression</b> impression taking on MultiPlus abutments on closed trays comprising: <ul style="list-style-type: none"><li>• MultiPlus impression posts</li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57522		L8	MultiPlus System	1
	57554		L12	MultiPlus System	1
					
<b>MultiPlus open-tray impression</b> impression taking on MultiPlus abutments on open trays comprising: <ul style="list-style-type: none"><li>• MultiPlus impression posts</li><li>• titanium screws L11 and L16</li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57523		L8	MultiPlus System	1
					

Implant analogs					
Description	REF	Color code	Size	Compatibility	Units
<b>MultiPlus implant analogs</b>	57524			MultiPlus System	1
	57525			MultiPlus System	4
					

<sup>4</sup> DIM analogs®					
Description	REF	Color code	Size	Compatibility	Units
<b>BEG MU 5.DIM</b>	549528			MultiPlus System	1
					

**Note:** Manufacturer notes about trade names, see page 111.

\*<sup>1</sup> Version of the BEGO Semados® RI implants, with Platform Switch design

\*<sup>2</sup> For torque specifications, see page 114

\*<sup>5</sup> Platform Switch design

## Multi<sup>Plus</sup> restoration

CAD positioner					
Description	REF	Color code	Size	Compatibility	Units
<b>CADP Multi<sup>Plus</sup></b> • CAD positioner Multi <sup>Plus</sup> • secondary screw Multi <sup>Plus</sup> Material: Titanium grade 4 Tool: Hexagon screwdriver 1.25mm *2	58255			Multi <sup>Plus</sup> System	1
					
Titanium abutment					
Description	REF	Color code	Size	Compatibility	Units
<b>Multi<sup>Plus</sup> titanium abutment</b> comprising: • Multi <sup>Plus</sup> titanium abutment • secondary screw Multi <sup>Plus</sup> • technician screw Multi <sup>Plus</sup> Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25mm *2	57526		L11	Multi <sup>Plus</sup> System	1
					
Universal abutment					
Description	REF	Color code	Size	Compatibility	Units
<b>Multi<sup>Plus</sup> Universal</b> comprising: • Multi <sup>Plus</sup> wax-up sleeve Universal • secondary screw Multi <sup>Plus</sup> • technician screw Multi <sup>Plus</sup> Material: Polyoxymethylene (POM) Tool: Hexagon screwdriver 1.25mm *2	57538		L11	Multi <sup>Plus</sup> System	1
					
<b>Internal reamer Multi<sup>Plus</sup></b> For re-working the internal form fit, incl. reamer handle	57540			Multi <sup>Plus</sup> System	1
					
<b>External reamer Multi<sup>Plus</sup></b> For re-working the external form fit, incl. reamer handle	57539			Multi <sup>Plus</sup> System	1
					

**Crown restoration Ø 3.75–5.5**

Easy-Con abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>PS Easy-Con</b> Material: Titanium alloy with TiN coating Tool: Insert tool <sup>3</sup> Locator® * <sup>2</sup>	58130	■	L1	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.75	1
	58131	■	L2	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.75	1
	58132	■	L3	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.75	1
	58133	■	L4	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.75	1
	58134	■	L1	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58135	■	L2	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58136	■	L3	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58137	■	L4	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58138	■	L1	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	58139	■	L2	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	58140	■	L3	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	58141	■	L4	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	58142	■	L2	SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1
	58143	■	L4	SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	1
<b>Insert tool Easy-Con / <sup>3</sup>Locator® with ratchet connection</b>	57008				1



Easy-Con impression taking					
Description	REF	Color code	Size	Compatibility	Units
<b>Easy-Con impression coping</b> Impression on Easy-Con	57751				4
<b>Easy-Con analog</b>	57760				4



**Note:** Manufacturer notes about trade names, see page 111.

\*<sup>1</sup> Version of the BEGO Semados® RI implants, with Platform Switch design

\*<sup>2</sup> For torque specifications, see page 114

\*<sup>5</sup> Platform Switch design

## Crown restoration Ø 3.75–5.5

Easy-Con female parts					
Description	REF	Color code	Size	Compatibility	Units
<b>Easy-Con laboratory set comprising:</b> <ul style="list-style-type: none"><li>• retention insert transparent, pink and blue</li><li>• block-out ring</li><li>• retention cap</li><li>• production insert, black</li></ul> Material: Titanium alloy / polyamide (PA12) Tool: Easy-Con instrument	57752				2
<b>Easy-Con instrument</b> For screw-fitting, removing, and repositioning the retention inserts, insertion aid for Easy-Con abutment	57753				1
<b>Easy-Con production insert (black)</b> Material: Polyamide (PA12)	57754				4
<b>Easy-Con retention insert (blue)</b> Withdrawal force approx.: 917g; 9N; 0°–10°   Material: Polyamide (PA12)	57755				4
<b>Easy-Con retention insert (pink)</b> Withdrawal force approx.: 1427g; 14N; 0°–10°   Material: Polyamide (PA12)	57756				4
<b>Easy-Con retention insert (transparent)</b> Withdrawal force approx.: 2243g; 22N; 0°–10°   Material: Polyamide (PA12)	57757				4
<b>Easy-Con retention insert (red)</b> Withdrawal force approx.: 663g; 6.5N; 10°–20°   Material: Polyamide (PA12)	57758				4
<b>Easy-Con retention insert (green)</b> Withdrawal force approx.: 2599g; 25.5N; 10°–20°   Material: Polyamide (PA12)	57759				4

Watch the video “BEGO Semados® Easy-Con System (chairside)”: <https://www.youtube.com/watch?v=JyfjwvzDQIY>



Watch the video “BEGO Semados® Easy-Con System (laboratory)”: <https://www.youtube.com/watch?v=JyfjwvzDQIY>



## Crown restoration Ø 3.25–4.5

Ball attachment abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>PS BA</b> comprising: <ul style="list-style-type: none"><li>• PS ball attachment without female parts</li><li>• spacer</li></ul> Material: Titanium alloy Tool: Insert tool Ball attachment <sup>*2</sup>	58120		GH 0	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	58121		GH 3	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	58122		GH 5	SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75	1
	58123		GH 0	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58124		GH 3	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58125		GH 5	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	1
	58126		GH 0	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	58127		GH 3	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
	58128		GH 5	SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	1
Insert tool for ball attachment with ratchet connection	55880				1



Impression set					
Description	REF	Color code	Size	Compatibility	Units
<b>Ball attachment impression set <sup>2</sup>Dalbo®-PLUS</b> impression on ball attachment comprising: <ul style="list-style-type: none"><li>• impression post cap for ball attachment (red)</li><li>• implant analog for ball attachment</li></ul>	55768				1



Ball attachment female parts <sup>2</sup> Dalbo®					
Description	REF	Color code	Size	Compatibility	Units
<b>Female parts <sup>2</sup>Dalbo®-PLUS</b> comprising: <ul style="list-style-type: none"><li>• female parts <sup>2</sup>Dalbo®-PLUS, complete (incl. retention insert)</li><li>• placeholder</li></ul> Material: Titanium grade 4 Tool: <sup>2</sup> Dalbo®-PLUS activator/de-activator	55769				1
<b>Activator/Deactivator <sup>2</sup>Dalbo®-PLUS</b>	55773				1
<b>Retention insert <sup>2</sup>Dalbo®-PLUS</b> Material: Precious metal Tool: <sup>2</sup> Dalbo®-PLUS activator/de-activator	55776				1



Watch the video "BEGO Semados® Ball Attachment":



## Screws

Prosthesis screws					
Description	REF	Color code	Size	Compatibility	Units
Prosthesis screw Hex 1.25mm	53999			Healing abutments, individual Ø 7, PS CADP, PS PPA, PS TPA, PS GCO / PS GCO NH	1
Prosthesis screw Sub-Tec <sup>Plus</sup>	57031			CAD SP, PS CATi, PS OCP, PS PMB, PS TiB / PS TiB NH, PS TTiA / PS TTiA NH, PS TiAA, PS TiA	1
Secondary screw Multi <sup>Plus</sup> (M1.4)	57534			Multi <sup>Plus</sup> System	1
Prosthesis screw Multi <sup>Plus</sup> (M1.8)	57535			PS Multi <sup>Plus</sup> 20° / 30°	1
PScrew	57782	<input type="checkbox"/>		Prosthesis Ø 3.0	1
PScrew	57784	<input type="checkbox"/>		CAD positioner Ø 3.0	1
PS UNI PScrew	57993			PS UNI / PS UNI NH	1

**Note:** Manufacturer notes about trade names, see page 111.

\*<sup>1</sup> Version of the BEGO Semados® RI implants, with Platform Switch design

\*<sup>2</sup> For torque specifications, see page 114

\*<sup>5</sup> Platform Switch design

---

<sup>\*7</sup> Platform Match design



## OVERVIEW

CAD/CAM restoration	92
Impression taking and model fabrication	94
Crown and bridge restoration	95
Multi <sup>Plus</sup> restoration	100
Hybrid restoration	104
Screws	107

## CAD/CAM restoration

CAD positioner					
Description	REF	Color code	Size	Compatibility	Units
<b>Sub-Tec CAD positioner</b> comprising: <ul style="list-style-type: none"><li>• Sub-Tec CAD positioner</li><li>• prosthesis screw Hex 1.25mm</li></ul> Material: Titanium grade 4 Tool: Hexagon screwdriver 1.25mm *2	57060			S/RI 3.25–5.5	1



Adhesive abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>Sub-Tec CAD/CAM titanium adhesive abutment</b> comprising: <ul style="list-style-type: none"><li>• Sub-Tec adhesive abutment</li><li>• prosthesis screw Sub-Tec<sup>Plus</sup></li><li>• technician screw Sub-Tec<sup>Plus</sup></li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57285			S/RI 3.25–3.75	1
	57287			S/RI 4.1	1
	57289			S/RI 4.5	1
	57291			S/RI 5.5	1
<b>Sub-Tec CAD/CAM titanium adhesive abutment no Hex</b> comprising: <ul style="list-style-type: none"><li>• Sub-Tec adhesive abutment no Hex</li><li>• prosthesis screw Sub-Tec<sup>Plus</sup></li><li>• technician screw Sub-Tec<sup>Plus</sup></li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57286			S/RI 3.25–3.75	1
	57288			S/RI 4.1	1
	57290			S/RI 4.5	1
	57292			S/RI 5.5	1



**Note:** When using the \*<sup>6</sup>Cerec® system, a \*<sup>6</sup>Cerec / \*<sup>6</sup>InLab scanbody for \*<sup>6</sup>Blucam (36 units) REF 6431303 or a scanbody for \*<sup>6</sup>Omnicam (36 units) REF 6431329 (Sirona Dental Systems GmbH, Bensheim, Germany) is required.

**Note:** For the ST PMB a \*<sup>6</sup>PreFace® abutment holder for the corresponding milling system is required. This must be ordered directly from the machine manufacturer. Please note the manufacturer's information regarding this!

\*<sup>1</sup> Version of the BEGO Semados® RI implants, with Platform Switch design

\* For torque specifications, see page 114

\*<sup>6</sup> This symbol is a commercial name/registered trademark of a company that does not belong to the BEGO Group.

\*<sup>7</sup> Platform Match design

## CAD/CAM restoration

Adhesive abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>Sub-Tec CAD/CAM TiBase L</b> comprising: <ul style="list-style-type: none"><li>• Sub-Tec TiBase</li><li>• prosthesis screw Sub-Tec<sup>Plus</sup></li><li>• technician screw Sub-Tec<sup>Plus</sup></li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57656			S/RI 3.25–3.75	1
	57657			S/RI 4.1	1
	57658			S/RI 4.5	1
	57659			S/RI 5.5	1

Scansupport					
Description	REF	Color code	Size	Compatibility	Units
<b>CAD SP</b> comprising: <ul style="list-style-type: none"><li>• scansupport</li><li>• prosthesis screw Sub-Tec<sup>Plus</sup></li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	58191			S/SC/SCX/RS/RSX/RI 3.25–3.75	1
	58192			S/SC/SCX/RS/RSX/RI 4.1	1
	58193			S/SC/SCX/RS/RSX/RI 4.5	1
	58194			S/SC/SCX/RS/RSX/RI 5.5	1

Milling blanks					
Description	REF	Color code	Size	Compatibility	Units
<b>ST PMB</b> comprising: <ul style="list-style-type: none"><li>• milling blank</li><li>• prosthesis screw Sub-Tec<sup>Plus</sup></li><li>• technician screw Sub-Tec<sup>Plus</sup></li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	58319		Ø11.5	S/RI 3.25–5.5	1
	58219		Ø16	S/RI 3.25–5.5	1



## Impression taking and model fabrication

Impression sets					
Description	REF	Color code	Size	Compatibility	Units
<b>Sub-Dent closed-tray impression</b> Impression taking on implant with closed tray comprising: <ul style="list-style-type: none"><li>• impression post cap</li><li>• sub impression posts</li><li>• titanium screw L11</li></ul> Tool: Hexagon screwdriver 1.25mm *2	55860	■	S	3.25	1
	55539	■	S/RI	3.75	1
	55617	■	S/RI	4.1	1
	55618	■	S/RI	4.5	1
	55551	■	S/RI	5.5	1



Implant analogs					
Description	REF	Color code	Size	Compatibility	Units
<b>Model implants</b>	56694	■	S	3.25	1
	56695	■	S/RI	3.75	1
	56696	■	S/RI	4.1	1
	56698	■	S/RI	4.5	1
	56699	■	S/RI	5.5	1



<sup>4</sup> DIM analogs <sup>®</sup>					
Description	REF	Color code	Size	Compatibility	Units
<b>BEG 5.DIM</b>	549316	■■	S/RI	3.25–3.75	1
	549317	■	S/RI	4.1	1
	549318	■	S/RI	4.5	1
	549319	■	S/RI	5.5	1



**Note:** Manufacturer notes about trade names, see page 111.

\*2 For torque specifications, see page 114

\*7 Platform Match design

## Crown and bridge restoration

Provisional abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>Sub-Tec provisional abutment</b> solid abutment, plastic for provisional restorations comprising: <ul style="list-style-type: none"><li>• plastic abutment</li><li>• prosthesis screw Hex 1.25mm</li><li>• technician screw</li></ul> Material: Polyetheretherketone (PEEK) Tool: Hexagon screwdriver 1.25mm 1.25mm *2	55951		Ø 7	S/RI 3.25–5.5	1
<b>Sub-Tec provisional PEEK abutment</b> comprising: <ul style="list-style-type: none"><li>• plastic abutment</li><li>• prosthesis screw Hex 1.25mm</li><li>• technician screw</li></ul> Material: Polyetheretherketone (PEEK) Tool: Hexagon screwdriver 1.25mm 1.25mm *2	57494			S/RI 3.25–3.75	1
	57495			S/RI 4.1–4.5	1
<b>Sub-Tec provisional titanium abutment</b> comprising: <ul style="list-style-type: none"><li>• Sub-Tec provisional titanium abutment</li><li>• prosthesis screw Sub-Tec<sup>Plus</sup></li><li>• technician screw Sub-Tec<sup>Plus</sup></li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm 1.25mm *2	57304			S/RI 3.25–3.75	1
	57305			S/RI 4.1	1
	57306			S/RI 4.5	1
	57307			S/RI 5.5	1
<b>Sub-Tec provisional titanium abutment no Hex</b> comprising: <ul style="list-style-type: none"><li>• Sub-Tec provisional titanium abutment no Hex</li><li>• prosthesis screw Sub-Tec<sup>Plus</sup></li><li>• technician screw Sub-Tec<sup>Plus</sup></li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm 1.25mm *2	57300			S/RI 3.25–3.75	1
	57301			S/RI 4.1	1
	57302			S/RI 4.5	1
	57303			S/RI 5.5	1



## Crown and bridge restoration

Solid abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>Sub-Tec<sup>Plus</sup> titanium abutment comprising:</b>	57116		GH 1–2	S/RI 3.25–3.75	1
• titanium abutment	57117		GH 2.5–4	S/RI 3.25–3.75	1
• prosthesis screw Sub-Tec <sup>Plus</sup>	57120		GH 1–2	S/RI 4.1	1
• technician screw Sub-Tec <sup>Plus</sup>	57121		GH 2.5–4	S/RI 4.1	1
Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57124		GH 1–2	S/RI 4.5	1
	57125		GH 2.5–4	S/RI 4.5	1
	57128		GH 1–2	S/RI 5.5	1
	57129		GH 2.5–4	S/RI 5.5	1



\*2 For torque specifications, see page 114  
\*7 Platform Match design

## Crown and bridge restoration

Solid abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>Sub-Tec<sup>Plus</sup> titanium angulated abutment</b> angle over plane (type P) or edge (type E) comprising: • angulated abutment • prosthesis screw Sub-Tec <sup>Plus</sup> • technician screw Sub-Tec <sup>Plus</sup> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57132	■■	15° P GH 1–2	S/RI 3.25–3.75	1
	57133	■■	15° P GH 2.5–4	S/RI 3.25–3.75	1
	57134	■■	15° E GH 1–2	S/RI 3.25–3.75	1
	57135	■■	15° E GH 2.5–4	S/RI 3.25–3.75	1
	57136	■■■	15° P GH 1–2	S/RI 4.1	1
	57137	■■■	15° P GH 2.5–4	S/RI 4.1	1
	57138	■■■	15° E GH 1–2	S/RI 4.1	1
	57139	■■■	15° E GH 2.5–4	S/RI 4.1	1
	57140	■■■■■	15° P GH 1–2	S/RI 4.5	1
	57141	■■■■■	15° P GH 2.5–4	S/RI 4.5	1
	57142	■■■■■	15° E GH 1–2	S/RI 4.5	1
	57143	■■■■■	15° E GH 2.5–4	S/RI 4.5	1
	57144	■■■■■■	15° P GH 1–2	S/RI 5.5	1
	57145	■■■■■■	15° P GH 2.5–4	S/RI 5.5	1
	57146	■■■■■■	15° E GH 1–2	S/RI 5.5	1
	57147	■■■■■■	15° E GH 2.5–4	S/RI 5.5	1



### Angulated abutment, type P

Type P = angle over plane



### Angulated abutment, type E

Type E = angle over edge



## Crown and bridge restoration

Universal abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>Sub-Tec Universal</b> comprising: <ul style="list-style-type: none"><li>• Universal base Hex</li><li>• sub wax-up sleeve Universal</li><li>• prosthesis screw</li><li>Sub-Tec Universal</li><li>• technician screw</li><li>Sub-Tec Universal (black)</li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	55525			S/RI 3.25–3.75	1
	55622			S/RI 4.1	1
	55527			S/RI 4.5	1
	55529			S/RI 5.5	1
<b>Sub-Tec Universal no Hex</b> comprising: <ul style="list-style-type: none"><li>• Universal base no Hex</li><li>• sub wax-up sleeve Universal</li><li>• prosthesis screw</li><li>Sub-Tec Universal</li><li>• technician screw</li><li>Sub-Tec Universal (black)</li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	55526			S/RI 3.25–3.75	1
	55623			S/RI 4.1	1
	55528			S/RI 4.5	1
	55530			S/RI 5.5	1
<b>Internal reamer Universal</b> For re-working the internal form fit	55536			S/SC/SCX/RS/RSX/RI	3.25–5.5
<b>External reamer Universal</b> For re-working the external form fit	55537			S/SC/SCX/RS/RSX/RI	3.25–5.5

Watch the video "BEGO Semados® Universal Abutment":



Watch the video "BEGO Semados® Universal Abutment no Hex":



\*2 For torque specifications, see page 114

\*3 Alloy recommendation: Bio PontoStar® XL (BEGO, REF 61140)/Bio PontoStar® (BEGO, REF 61104)

\*7 Platform Match design

## Crown and bridge restoration

### Gold cast-on abutments

Description	REF	Color code	Size	Compatibility	Units	
<b>Sub-Tec gold cast-on comprising:</b> <ul style="list-style-type: none"><li>• sub cast-on abutment</li><li>• sub wax-up sleeve gold cast-on</li><li>• prosthesis screw Hex 1.25mm</li><li>• technician screw</li></ul> Material: Gold /platinum alloy Tool: Hexagon screwdriver 1.25mm *2 *3	55862	■■		S/RI 3.25–3.75	1	
	55624	■		S/RI 4.1	1	
	56317	■		S/RI 4.5	1	
<b>Sub-Tec gold cast-on no Hex comprising:</b> <ul style="list-style-type: none"><li>• sub cast-on abutment no Hex</li><li>• sub wax-up sleeve gold cast-on</li><li>• prosthesis screw Hex 1.25mm</li><li>• technician screw</li></ul> Material: Gold /platinum alloy Tool: Hexagon screwdriver 1.25mm *2 *3	55873	■■		S/RI 3.25–3.75	1	
	55625	■		S/RI 4.1	1	
	56325	■		S/RI 4.5	1	
	56515	■		S/RI 5.5	1	
<b>Internal reamer for gold cast-on abutment</b> For re-working the internal form fit (a technician screwdriver is recommended as the hold)	53735	■■■■■		S/SC/SCX/RS/RSX/RI	3.25–5.5	

## MultiPlus restoration

Auxiliary parts					
Description	REF	Color code	Size	Compatibility	Units
<b>MultiPlus insertion splint</b> To determine the planned angle	57532			MultiPlus System	1
<b>MultiPlus alignment aids</b> For aligning the implant hex	57530		20°	MultiPlus System	1
	57531		30°	MultiPlus System	1

Abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>Sub-Tec MultiPlus abutments</b> comprising: • Sub-Tec MultiPlus abutment 0° • MultiPlus positioning aid 0° Material: Titanium alloy (packaged sterile) Tool: Insertion instrument MultiPlus abutment 0° *2	57505	■■	0° GH 1	S/RI 3.25–3.75	1
	58336*	■■	0° GH 2	S/RI 3.25–3.75	1
	57508	■■	0° GH 3	S/RI 3.25–3.75	1
	58516*	■■	0° GH 4	S/RI 3.25–3.75	1
	57506	■	0° GH 1	S/RI 4.1	1
	58337*	■	0° GH 2	S/RI 4.1	1
	57509	■	0° GH 3	S/RI 4.1	1
	58517*	■	0° GH 4	S/RI 4.1	1
	57507	■	0° GH 1	S/RI 4.5	1
	58338*	■	0° GH 2	S/RI 4.5	1
	57510	■	0° GH 3	S/RI 4.5	1
	58518*	■	0° GH 4	S/RI 4.5	1
<b>Insertion instrument</b> <b>MultiPlus abutment 0°</b> with ratchet connection	57533			MultiPlus System	1
<b>Insertion instrument</b> <b>MultiPlus abutment 0°</b> with contra-angle connection	58199			MultiPlus System	1

\* Planned availability from November 2021

\*2 For torque specifications, see page 114

\*7 Platform Match design

## Multi<sup>Plus</sup> restoration

Abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>Sub-Tec Multi<sup>Plus</sup> abutment</b> comprising: <ul style="list-style-type: none"><li>• Sub-Tec Multi<sup>Plus</sup> abutment 20°</li><li>• Multi<sup>Plus</sup> positioning aid 20°</li><li>• prosthesis screw Multi<sup>Plus</sup></li></ul> Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25mm *2	57511		20° GH 2.3–0.6	S/RI 3.25–3.75	1
	57514		20° GH 4.0–2.3	S/RI 3.25–3.75	1
	57512		20° GH 2.3–0.6	S/RI 4.1	1
	57515		20° GH 4.0–2.3	S/RI 4.1	1
	57513		20° GH 2.3–0.6	S/RI 4.5	1
	57516		20° GH 4.0–2.3	S/RI 4.5	1
<b>Sub-Tec Multi<sup>Plus</sup> abutment</b> comprising: <ul style="list-style-type: none"><li>• Sub-Tec Multi<sup>Plus</sup> abutment 30°</li><li>• Multi<sup>Plus</sup> positioning aid 30°</li><li>• prosthesis screw Multi<sup>Plus</sup></li></ul> Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25mm *2	57517		30° GH 4.0–1.5	S/RI 3.25–3.75	1
	57518		30° GH 4.0–1.5	S/RI 4.1	1
	57519		30° GH 4.0–1.5	S/RI 4.5	1



Healing posts					
Description	REF	Color code	Size	Compatibility	Units
<b>Multi<sup>Plus</sup> healing post</b> prefabricated gingival former Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25mm	57520		L5	Multi <sup>Plus</sup> System	1
<b>Multi<sup>Plus</sup> healing post</b> <b>Mushroom</b> prefabricated gingival former Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25mm	57521		L5	Multi <sup>Plus</sup> System	1



## MultiPlus restoration

Impression sets					
Description	REF	Color code	Size	Compatibility	Units
<b>MultiPlus closed-tray impression</b> impression taking on MultiPlus abutments on closed trays comprising: <ul style="list-style-type: none"><li>• MultiPlus impression posts</li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57522		L8	MultiPlus System	1
	57554		L12	MultiPlus System	1
					
<b>MultiPlus open-tray impression</b> (impression taking on MultiPlus abutments on open trays) comprising: <ul style="list-style-type: none"><li>• MultiPlus impression posts</li><li>• titanium screws L11 and L16</li></ul> Material: Titanium alloy Tool: Hexagon screwdriver 1.25mm *2	57523		L8	MultiPlus System	1
					
Implant analogs					
Description	REF	Color code	Size	Compatibility	Units
<b>MultiPlus implant analogs</b>	57524			MultiPlus System	1
	57525			MultiPlus System	4
					
<sup>4</sup> DIM-Analogs®					
Description	REF	Color code	Size	Compatibility	Units
<b>BEG MU 5.DIM</b>	549528			MultiPlus System	1
					

**Note:** Manufacturer notes about trade names, see page 111.

\*2 For torque specifications, see page 114

\*7 Platform Match design

## Multi<sup>Plus</sup> restoration

CAD positioner					
Description	REF	Color code	Size	Compatibility	Units
<b>CADP Multi<sup>Plus</sup></b> • CAD positioner Multi <sup>Plus</sup> • secondary screw Multi <sup>Plus</sup> Material: Titanium grade 4 Tool: Hexagon screwdriver 1.25mm *2	58255			Multi <sup>Plus</sup> System	1
					
Titanium abutment					
Description	REF	Color code	Size	Compatibility	Units
<b>Multi<sup>Plus</sup> titanium abutment</b> comprising: • Multi <sup>Plus</sup> titanium abutment • secondary screw Multi <sup>Plus</sup> • technician screw Multi <sup>Plus</sup> Material: Titanium alloy (packaged sterile) Tool: Hexagon screwdriver 1.25mm *2	57526		L11	Multi <sup>Plus</sup> System	1
					
Universal abutment					
Description	REF	Color code	Size	Compatibility	Units
<b>Multi<sup>Plus</sup> Universal</b> comprising: • Multi <sup>Plus</sup> wax-up sleeve Universal • secondary screw Multi <sup>Plus</sup> • technician screw Multi <sup>Plus</sup> Material: Polyoxymethylene (POM) Tool: Hexagon screwdriver 1.25mm	57538		L11	Multi <sup>Plus</sup> System	1
					
<b>Internal reamer Multi<sup>Plus</sup></b> For re-working the internal form fit, incl. reamer handle	57540			Multi <sup>Plus</sup> System	1
					
<b>External reamer Multi<sup>Plus</sup></b> For re-working the external form fit, incl. reamer handle	57539			Multi <sup>Plus</sup> System	1
					

Watch the video “BEGO Semados® Multi<sup>Plus</sup> System”:



## Hybrid restoration

Easy-Con abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>Sub-Tec Easy-Con abutment</b> Material: Titanium alloy with TiN coating Tool: Insert tool <sup>3</sup> Locator® *2	57743	■■	L1	S/RI 3.75–4.1	1
	57744	■■	L2	S/RI 3.75–4.1	1
	57745	■■	L3	S/RI 3.75–4.1	1
	57746	■■	L4	S/RI 3.75–4.1	1
	57747	■	L1	S/RI 4.5	1
	57748	■	L2	S/RI 4.5	1
	57749	■	L3	S/RI 4.5	1
	57750	■	L4	S/RI 4.5	1
<b>Insert tool Easy-Con /</b> <sup>3</sup> Locator® with ratchet connection	57008				1



Easy-Con impression taking					
Description	REF	Color code	Size	Compatibility	Units
<b>Easy-Con impression coping</b> Impression on Easy-Con	57751				4
<b>Easy-Con analog</b>	57760				4



**Note:** Manufacturer notes about trade names, see page 111.

\*2 For torque specifications, see page 114

\*7 Platform Match design

## Hybrid restoration

Easy-Con female parts					
Description	REF	Color code	Size	Compatibility	Units
<b>Easy-Con laboratory set</b> comprising: • retention insert transparent, pink, and blue • block-out ring • retention cap • production insert, black Material: Titanium alloy / polyamide (PA12) Tool: Easy-Con instrument	57752				2
<b>Easy-Con instrument</b> For screw-fitting, removing, and repositioning the retention inserts, insertion aid for Easy-Con abutment	57753				1
<b>Easy-Con production insert (black)</b> Material: Polyamide (PA12)	57754				4
<b>Easy-Con retention insert (blue)</b> Withdrawal force approx.: 917g; 9N; 0–10°   Material: Polyamide (PA12)	57755				4
<b>Easy-Con retention insert (pink)</b> Withdrawal force approx.: 1427g; 14N; 0–10°   Material: Polyamide (PA12)	57756				4
<b>Easy-Con retention insert (transparent)</b> Withdrawal force approx.: 2243g; 22N; 0–10°   Material: Polyamide (PA12)	57757				4
<b>Easy-Con retention insert (red)</b> Withdrawal force approx.: 663g; 6.5N; 10–20°   Material: Polyamide (PA12)	57758				4
<b>Easy-Con retention insert (green)</b> Withdrawal force approx.: 2599g; 25.5N; 10–20°   Material: Polyamide (PA12)	57759				4

Watch the video “BEGO Semados® Easy-Con System (chairside)”: [\[QR code\]](#)



Watch the video “BEGO Semados® Easy-Con System (laboratory)”: [\[QR code\]](#)



## Hybrid restoration

Ball attachment abutments					
Description	REF	Color code	Size	Compatibility	Units
<b>Sub-Tec ball attachment</b> comprising: <ul style="list-style-type: none"><li>• sub ball attachment without female parts</li><li>• spacer</li></ul> Material: Titanium alloy Tool: Insert tool Ball attachment *2	57631 57633 57635 57632 57634 57636	     	GH 0 GH 3 GH 5 GH 0 GH 3 GH 5	S/RI 3.25–3.75 S/RI 3.25–3.75 S/RI 3.25–3.75 S/RI 4.1–4.5 S/RI 4.1–4.5 S/RI 4.1–4.5	1 1 1 1 1 1
Insert tool for ball attachment with ratchet connection	55880				1
Impression set					
Description	REF	Color code	Size	Compatibility	Units
<b>Ball attachment impression set <sup>2</sup>Dalbo®-PLUS</b> impression on ball attachment comprising: <ul style="list-style-type: none"><li>• impression post cap for ball attachment (red)</li><li>• implant analog for ball attachment</li></ul>	55768				1
Ball attachment female parts <sup>2</sup> Dalbo®					
Description	REF	Color code	Size	Compatibility	Units
<b>Female parts <sup>2</sup>Dalbo®-PLUS</b> comprising: <ul style="list-style-type: none"><li>• female parts <sup>2</sup>Dalbo®-PLUS, complete (incl. retention insert)</li><li>• placeholder</li></ul> Material: Titanium grade 4 Tool: <sup>2</sup> Dalbo®-PLUS activator/deactivator	55769				1
<b><sup>2</sup>Dalbo®-PLUS</b> activator/deactivator	55773				1
<b>Retention insert <sup>2</sup>Dalbo®-PLUS</b> Material: Precious metal Tool: <sup>2</sup> Dalbo®-PLUS activator/deactivator	55776				1

Watch the video "BEGO Semados® Ball Attachment":



\*2 For torque specifications, see page 114

\*7 Platform Match design

## Screws

Prosthesis screws						
Description	REF	Color code	Size	Compatibility	Units	
Prosthesis screw Hex 1.25mm	53999			Sub-Tec gold cast-on, Sub-Tec temporary abutment, Sub-Tec provisional PEEK abutment, Sub-Tec titanium abutment, Sub-Tec bar system (until Q2 2013), Sub-Tec CAD positioner, healing abutments, individual Ø 7	1	
Prosthesis screw Sub-Tec <sup>Plus</sup>	57031			CAD SP, ST PMB, Sub-Tec <sup>Plus</sup> abutments (straight and angled), Sub-Tec CAD/CAM titanium adhesive abutment, Sub-Tec provisional titanium abutment, Sub-Tec bar system (from Q2 2013), Sub-Tec CAD/CAM TiBase L	1	
Prosthesis screws Sub-Tec Universal	55534			Sub-Tec Universal	3.25–4.5	
	55535			Sub-Tec Universal	5.5	
Secondary screw Multi <sup>Plus</sup> (M1.4)	57534			Multi <sup>Plus</sup> System	1	
Prosthesis screw Multi <sup>Plus</sup> (M1.8)	57535			Sub-Tec Multi <sup>Plus</sup> 20/30°	1	





## OVERVIEW

Large-scale models

110

Demo material

111

## DEMO MODELS/MATERIAL

Large-scale models					
Description	REF	Color code	Size	Compatibility	Units
BEGO Semados® SCX implant large-scale model	58242				1
					
BEGO Semados® RSX implant large-scale model	58515				1
					
BEGO Semados® RI*¹ implant large-scale model	58322				1
					
Acrylic block PS (large-scale model, scale 2:1) comprising:	56753				1
• acrylic block					
• one SCX and one RSX implant Ø 4.1 L11.5					
• PS TTIA (temporary abutment)					
• PS TiB (adhesive abutment)					
• PS TiAA, 15° P GH 1–2 (solid abutment)					
• PS TiAA, 20° E GH 2.5–4 (solid abutment)					
• prosthesis screw					
• hex screwdriver					
					

\*¹ Version of the BEGO Semados® RI implants, with Platform Switch design

## DEMO MODELS/MATERIAL

### DEMO MODELS/MATERIAL

Demonstration material					
Description	REF	Color code	Size	Compatibility	Units
<b>Maxilla demonstration model</b> Clear acrylic model with implants	58243			SCX implants	1
	56755			RSX implants	1
<b>BEGO Semados® demo implants</b> incl. cover screw and titanium insertion post Material: Titanium (packaged non-sterile) Not for use on patients!	58244		SC		1
	58245		SCX		1
	58320		RS <sup>Pro</sup>		1
	58321		RSX <sup>Pro</sup>		1
	57699		RSX 3.0		1
	58345		RI* <sup>1</sup>		1
	55543		S		1
TJL (training jaw)	57464		Mandible		1
TJU (training jaw)	57465		Maxilla		1



**Note:**

<sup>2</sup>Dalbo® is a registered trademark of Cendres & Métaux SA, Biel/Bienne, Switzerland.

<sup>3</sup>Locator® is a registered trademark of ZEST Anchors LLC, CA, USA.

<sup>4</sup>DIM-Analog® is a registered trademark of nt-trading GmbH & Co. KG, Karlsruhe, Germany.





## OVERVIEW

Torque specifications	114
Material specifications	116
Index by article numbers	122
Alphabetical index	136

## USEFUL INFORMATION · TORQUE SPECIFICATIONS

Torques for BEGO Semados®	
Article name	Torque [Ncm]
Implant cover screw	10
Healing abutments	10
Healing abutments, individual	15
Impression post	10
CAD positioner (polyetheretherketone)	10
CAD positioner (grade 4 titanium)	15
CAD SP	15
<b>Temporary abutments</b>	<b>15</b>
• PS ITA Ø3.0–5.5 (temporary abutment) • PS PPA Ø3.25–5.5 (temporary abutment) • PS TPA Ø3.25–5.5 (temporary abutment) • PS TTiA/PS TTiA NH Ø3.25–5.5 (temporary abutment Hex/no Hex) • Sub-Tec temporary abutment (PEEK) • Sub-Tec provisional titanium abutment	
<b>Platform Switch System Ø3.0</b>	<b>20</b>
• PS TiA/PS TiAA Ø3.0 (solid abutment) • PS TiB Ø3.0 (adhesive abutment)	
<b>Platform Switch System Ø3.25–5.5</b>	<b>30</b>
• PS BA Ø3.25–4.5 (ball attachment abutment) • PS Easy-Con Ø3.75–4.5 (abutment) • PS PMB (milling blank, TI-Form milling blank) • PS TiB/PS TiB NH Ø3.25–5.5 (adhesive abutment Hex/no Hex) • PS OCP (restoration set) • PS GCO/PS GCO NH Ø3.25–5.5 (gold cast-on abutment Hex/no Hex) • PS Multi <sup>Plus</sup> Ø3.25–4.5 (post) • PS TiA/PS TiAA Ø3.75–5.5 (solid abutment) • PS UNI/PS UNI NH Ø3.25–5.5 (Universal abutment Hex/no Hex)	
<b>Platform Match System (Sub-System)</b>	<b>30</b>
• Sub-Tec ball attachment • Sub-Tec Easy-Con • ST PMB (milling blank) • Sub-Tec CAD/CAM TiBase L • Sub-Tec CAD/CAM titanium adhesive abutment • Sub-Tec gold cast-on • Sub-Tec Multi <sup>Plus</sup> abutment • Sub-Tec <sup>Plus</sup> titanium abutment • Sub-Tec Universal	
<b>Multi<sup>Plus</sup> System</b>	<b>20</b>
• Multi <sup>Plus</sup> titanium abutment • Multi <sup>Plus</sup> Universal	
<b>Mini System</b>	<b>25</b>
• Easy-Con Mini • Gold cast-on Mini • Ball attachment Mini • TiA (solid abutment) • TiBA (bar abutment)	

**Note:** Manufacturer notes about trade names, see page 111.

## General notes

To prevent damage to the components, original BEGO Implant Systems tools and products must be used for processing. The use of the torque ratchet in particular is required to comply with the prescribed initial tension of the connecting screws (specification stated in Ncm).

- Ensure that the prosthesis screws are not used in the laboratory and check that they have not been damaged.
- Once the implant abutments are finally screwed in, after about 5 to 10 minutes all connecting screws must be tightened/checked once more with the specified tightening torque.
- The implant/prosthesis interfaces must be regularly checked to ensure they are firmly seated and there are no gaps.
- If the components are exposed to extremely high loads, the screw(s) may loosen under some circumstances. The reasons for this must be identified and eliminated!
- It is recommended that implant abutments that are screwed in the implant with a separate prosthesis screw are screwed in with a new prosthesis screw if the screw is loosened, for example, for cleaning the prosthetic restoration/implant abutments.

All specifications are determined to the best of our knowledge based on many years of practical applications and apply for restorations that have been executed in accordance with both our expertise and general scientific knowledge.

## General information about titanium

Titanium is a biopassive or bioinert substance that has an exceptionally neutral taste and is radiotransparent and resistant to corrosion as well as being a poor conductor of heat (thermal conductivity 0.168 to gold 3.118).

In implant dentistry, pure titanium and titanium alloys are processed while pure titanium also contains foreign components. Pure titanium is classified into 4 grades based on the proportion of foreign substances.

In all 4 groups, a maximum of 0.05% N, 0.08% C, and 0.015% H may be present. These substances are unavoidable because they are produced during the extraction of titanium or are deliberately introduced to control the physical properties.

Pure titanium (grades 1–4) and titanium alloys (from grade 5 onward) can be used for all dental work. It is possible to veneer crowns and bridges made of titanium with special ceramics, which, because of a phase transformation of the titanium at 882 °C (volume change), are fired at temperatures below 800 °C and must have a specific WAK (titanium: WAK of approx. 9.6).

When processing and polishing, the poor thermal conductivity of titanium must be heeded. During processing, heat may accumulate in localized areas, leading to increased O<sub>2</sub> deposits and in turn to embrittlement of the material.

Because titanium smears during machining, special mills must be used. Freshly polished surfaces only retain their mirror finish if they do not come into contact with H<sub>2</sub>O for at least 10 minutes.

During this time, they form a surface oxide that acts as a protective layer. When modelling frameworks, it must be noted that when casting titanium a thick, strong oxide layer develops with components of the investment material, which is known as the  $\alpha$  cast layer. This layer must be removed leaving no residue. Edges of models must be reinforced and are adjusted during the finishing. Titanium and titanium alloys can only be joined using welding (laser, plasma, arc, resistance).

Titanium				
Elements	Grade 2	Grade 3	Grade 4	Grade 5
Nitrogen, max. [%]	0.03	0.05	0.05	0.05
Carbon, max. [%]	0.08	0.08	0.08	0.08
Hydrogen, max. [%]	0.015	0.015	0.015	0.015
Iron, max. [%]	0.3	0.3	0.5	0.4
Oxygen, max. [%]	0.25	0.35	0.4	0.2
Aluminum [%]				5.5–6.75
Vanadium [%]				3.5–4.5
Titanium [%]	Remainder	Remainder	Remainder	Remainder

Compositions	
Material	Article
<b>Pure titanium grade 4</b> As per ASTM F67	BEGO Semados® S/SC/SCX/RS/RSX/RI/Mini implants CADP/CADP Multi <sup>Plus</sup> (CAD positioner) Implant cover screws Female parts <sup>2</sup> Dalbo®-PLUS, female parts PS CADP (CAD positioner) Sub-Tec CAD positioner TiBA (bar abutment)
<b>Titanium grade 5</b> (titanium alloy Ti-6Al-4V) As per ASTM F136	Impression post Healing abutment Selection set 0°/15°/20° BEGO Guide master sleeves/spoons BEGO Semados® Provisional Implant (PI) BEGO Semados® insertion posts on implants CAD SP (scansupport) Drill stops Easy-Con impression coping – cap, analog, retention cap Easy-Con Mini (titanium-nitride coating) Ball attachment Mini Model implants S/RS/RSX/RI/Mini Multi <sup>Plus</sup> healing posts, impressions, implant analogs, titanium abutment OCP A (implant analogs) Open-tray impression for Mini, Mini impression post PI bending tool, PI implant analog, PI multifunctional cap, PI paralleling post Prosthesis screws/technician screws PS BA (ball attachment abutment) PS BA (ball attachment abutment), spacer PS Easy-Con (abutment) (titanium-nitride coating) PS HP/PS HPW (healing abutment) PS ITA (temporary abutment) PS Multi <sup>Plus</sup> (post) PS OCP, OCP abutment (restoration set)

## USEFUL INFORMATION · MATERIAL SPECIFICATIONS

Compositions	
Material	Article
<b>Titanium grade 5</b> (titanium alloy Ti-6Al-4V) As per ASTM F136	DIM-Analog® body IDC (implant adjustment instrument) PS PMB (milling blank, TI-Form milling blank) PS TiA (solid abutments) PS TiAA (solid abutments) PS TiB/PS TiB NH (adhesive abutment) PS TTIA/PS TTIA NH (temporary abutment) PS UNI/PS UNI NH (Universal abutment Hex/no Hex), Universal base Hex/no Hex ST PMB (milling blank) Sub-Tec CAD/CAM TiBase L Sub-Tec CAD/CAM titanium adhesive abutment Hex/no Hex Sub-Tec Easy-Con abutment (titanium-nitride coating) Sub-Tec ball attachment Sub-Tec ball attachment, spacer Sub-Tec MultiPlus abutment Sub-Tec Universal/no Hex, Universal base Hex/no Hex Sub-TecPlus titanium abutment/titanium angulated abutment TiA (solid abutment)
<b>Stainless steel</b>	BEGO Guide preparation instruments/instruments, initial drills, tissue punches, bone shapers, pilot drills, pilot markers, depth drills, countersinks, threadformers, thread taps, shape drills, trepan drills DIM-Analog® knurled screw Paralleling post S/RS/RSX/RI/Mini Insert tool for implants Depth gauge Guiding wrench Drill extension PI removal tool/insert tool/stabilizer
<b>Polyetheretherketone (PEEK)</b>	Healing abutment, individual Ø 7 PI protection cap PS OCP (restoration set), multifunctional cap PS PPA/PS TPA (temporary abutment) Sub-Tec temporary abutment Ø 7, Sub-Tec provisional PEEK abutment
<b>60Au-19Pt-20Pd-1Ir</b>	Gold cast-on Mini, cast-on abutment Mini PS GCO/PS GCO NH (gold cast-on abutment Hex/no Hex), cast-on abutment Hex/no Hex Sub-Tec gold cast-on/no Hex, sub-cast-on abutment/no Hex
<b>69Au-12Ag-11Cu-4Pd-3Pt</b>	Female parts <sup>2</sup> Dalbo®-PLUS, retention insert <sup>2</sup> Dalbo-PLUS <sup>2</sup> Dalbo®-PLUS

**Note:** Manufacturer notes about trade names, see page 111.

**Compositions**

Material	Article
<b>Polyoxymethylene (POM)</b>	Female parts <sup>2</sup> Dalbo®-PLUS, placeholder
	Multi <sup>Plus</sup> Universal, wax-up sleeve for gold cast-on
	PS CTI (impression set, closed tray), impression post cap
	PS UNI/PS UNI NH (Universal abutment Hex/no Hex), wax-up sleeve Universal
	Sub-Dent closed-tray impression, impression post cap
	Sub-Tec Universal/no Hex, sub-wax-up sleeve Universal
<b>Polycarbonate (PC)</b>	LCC, LCB (laboratory caps)
	PS GCO/PS GCO NH (gold cast-on abutment Hex/no Hex), wax-up sleeve for gold cast-on
	Sub-Tec gold cast-on/no Hex, sub-wax-up sleeve gold cast-on
<b>Polyamide (PA)</b>	Easy-Con impression coping, production insert
	Easy-Con retention insert

## NOTES



## INDEX · PRODUCTS BY ARTICLE NUMBERS

REF	Article	Page	REF	Article	Page
53735	Internal reamer for gold cast-on abutment	81, 99	55624	Sub-Tec gold cast-on, S/RI 4.1	99
53872	Depth gauge, S/SC/SCX	59	55625	Sub-Tec gold cast-on no Hex, S/RI 4.1	99
53888	Radiographic template, S implants	20	55715	Drill stops, S/SC/SCX 4.1	52
53897	Guiding wrench	58	55745	Radiographic template, RI implants	20
53948	Hexagon screwdriver 1.25mm, long, with ratchet connection	62	55746	Depth gauge, RI	59
53949	Hexagon screwdriver 1.25mm, short, with ratchet connection	62	55766	Threadformer, RI 3.25	57
53952	Slot screwdriver, long with ratchet connection	62	55768	Ball attachment impression set Dalbo®-PLUS	88, 106
53999	Prosthesis screw Hex 1.25mm	89, 107	55769	Female parts Dalbo®-PLUS	88, 106
55505	Implant cover screw, S 3.25	40	55773	Activator/deactivator Dalbo®-PLUS	88, 106
55525	Sub-Tec Universal, S/RI 3.25–3.75	98	55776	Retention insert Dalbo®-PLUS	88, 106
55526	Sub-Tec Universal no Hex, S/RI 3.25–3.75	98	55799	Ratchet/torque wrench	59, 62
55527	Sub-Tec Universal, S/RI 4.5	98	55804	Drill stops, depth drill 2.5 and S/SC/SCX 3.25–3.75	52
55528	Sub-Tec Universal no Hex, S/RI 4.5	98	55810	Drill stops, S/SC/SCX 4.5	51
55529	Sub-Tec Universal, S/RI 5.5	98	55815	Trepan drill, Ø5.0 external/Ø4.1 internal	59
55530	Sub-Tec Universal no Hex, S/RI 5.5	98	55816	Trepan drill, Ø6.0 external/Ø5.1 internal	59
55534	Prosthesis screw Sub-Tec Universal, S/RI 3.25–4.5	107	55817	Trepan drill, Ø4.2 external/Ø3.7 internal	59
55535	Prosthesis screw Sub-Tec Universal, S/RI 5.5	107	55826	Prosthetic kit	62
55536	Internal reamer Universal	80, 98	55830	Insert tool for implants, long, with ratchet connection	58
55537	External reamer Universal	80, 98	55831	Insert tool for implants, short, with ratchet connection	58
55539	Sub-Dent closed-tray impression, S/RI 3.75	94	55832	Insert tool for implants, long, with contra-angle connection	58
55540	Sub-Dent open-tray impression, S/RI 3.75	94	55860	Sub-Dent closed-tray impression, S 3.25	94
55543	BEGO Semados® S demo implants	111	55861	Sub-Dent open-tray impression, S 3.25	94
55551	Sub-Dent closed-tray impression, S/RI 5.5	94	55862	Sub-Tec gold cast-on, S/RI 3.25–3.75	99
55563	Hexagon screwdriver 1.25mm, short, contra-angle	62	55863	Paralleling post, S/SC/SCX	58
55564	Hexagon screwdriver 1.25mm, long, contra-angle	62	55873	Sub-Tec gold cast-on no Hex, S/RI 3.25–3.75	99
55590	Healing abutment, Ø4.0 L3, S/RI 3.25–3.75	40	55880	Insert tool for ball attachment	88, 106
55591	Healing abutment, Ø4.0 L5, S/RI 3.25–3.75	40	55908	Implant cover screw, S/RI 5.5	40
55592	Healing abutment, Ø4.0 L7, S/RI 3.25–3.75	40	55910	Drill stops, S/SC/SCX 5.5	52
55593	Healing abutment, Ø5.0 L3, S/RI 3.25–4.5	40	55951	Sub-Tec temporary abutment Ø7, S/RI 3.25–5.5	95
55594	Healing abutment, Ø5.0 L5, S/RI 3.25–4.5	40	55953	Healing abutment, individual Ø7, S/SC/SCX/RS/RSX/RI 3.25–5.5	35, 40
55595	Healing abutment, Ø5.0 L7, S/RI 3.25–4.5	40	56300	Healing abutment, Ø4.5 L3, S/RI 3.25–4.5	40
55599	BEGO Semados® ratchet adapter	59, 62	56301	Healing abutment, Ø4.5 L5, S/RI 3.25–4.5	40
55608	Implant cover screw, S/RI 3.75	40	56302	Healing abutment, Ø4.5 L7, S/RI 3.25–4.5	40
55615	Implant cover screw, S/RI 4.1	40	56303	Healing abutment, Ø6.0 L3, S/RI 3.25–5.5	40
55616	Implant cover screw, S/RI 4.5	40	56304	Healing abutment, Ø6.0 L5, S/RI 3.25–5.5	40
55617	Sub-Dent closed-tray impression, S/RI 4.1	94	56305	Healing abutment, Ø6.0 L7, S/RI 3.25–5.5	40
55618	Sub-Dent closed-tray impression, S/RI 4.5	94	56317	Sub-Tec gold cast-on, S/RI 4.5	99
55619	Sub-Dent open-tray impression, S/RI 4.1	94	56325	Sub-Tec gold cast-on no Hex, S/RI 4.5	99
55620	Sub-Dent open-tray impression, S/RI 4.5	94	56500	Sub-Dent open-tray impression, S/RI 5.5	94
55622	Sub-Tec Universal, S/RI 4.1	98			
55623	Sub-Tec Universal no Hex, S/RI 4.1	98			

**Note:** Manufacturer notes about trade names, see page 111.

## INDEX · PRODUCTS BY ARTICLE NUMBERS

REF	Article	Page	REF	Article	Page
56515	Sub-Tec gold cast-on no Hex, S/RI 5.5	99	57133	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° GH 2.5–4, S/RI 3.25–3.75	97
56694	Model implant, 3.25	94	57134	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 1–2, S/RI 3.25–3.75	97
56695	Model implant, S/RI 3.75	94	57135	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 2.5–4, S/RI 3.25–3.75	97
56696	Model implant, S/RI 4.1	94	57136	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° P GH 1–2, S/RI 4.1	97
56698	Model implant, S/RI 4.5	94	57137	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° P GH 2.5–4, S/RI 4.1	97
56699	Model implant, S/RI 5.5	94	57138	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 1–2, S/RI 4.1	97
56748	IDC, S/SC/SCX/RS/RSX/RI 3.25–5.5 (adjustment instrument)	58	57139	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 2.5–4, S/RI 4.1	97
56749	IDC, RS/RSX 3.0 (adjustment instrument)	58	57140	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° P GH 1–2, S/RI 4.5	97
56751	BEGO Semados® RS demo implants	111	57141	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° P GH 2.5–4, S/RI 4.5	97
56752	BEGO Semados® RSX demo implants	111	57142	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 1–2, S/RI 4.5	97
56753	Acrylic block PS (large-scale model, scale 2:1)	110	57143	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 2.5–4, S/RI 4.5	97
56755	Maxilla demonstration model, RSX implants	111	57144	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° P GH 1–2, S/RI 5.5	97
56990	Insert tool for implants, short, with contra-angle connection	58	57145	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° P GH 2.5–4, S/RI 5.5	97
56991	Trepan drill, Ø 5.0 external / Ø 4.3 internal	59	57146	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 1–2, S/RI 5.5	97
57008	Insert tool Easy-Con/Locator®	86, 104	57147	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 2.5–4, S/RI 5.5	97
57031	Prosthesis screw Sub-Tec <sup>Plus</sup>	89, 107	57265	Drill extension, one-part (without internal cooling)	58
57060	Sub-Tec CAD positioner, S/RI 3.25–5.5	92	57266	Hexagon screwdriver 1.25mm XS, with ratchet connection	62
57100	Depth drill 2.5, short S/SC/SCX	51	57285	Sub-Tec CAD/CAD titanium adhesive abutment, S/RI 3.25–3.75	92
57101	Depth drill 2.5, long S/SC/SCX	51	57286	Sub-Tec CAD/CAM titanium adhesive abutment no Hex, S/RI 3.25–3.75	92
57102	Depth drill, short S/SC/SCX 3.25	51	57287	Sub-Tec CAD/CAD titanium adhesive abutment, S/RI 4.1	92
57103	Depth drill, long S/SC/SCX 3.25	51	57288	Sub-Tec CAD/CAM titanium adhesive abutment no Hex, S/RI 4.1	92
57104	Depth drill, short S/SC/SCX 3.75	51	57289	Sub-Tec CAD/CAM titanium adhesive abutment, S/RI 4.5	92
57105	Depth drill, long S/SC/SCX 3.75	51			
57106	Depth drill, short S/SC/SCX 4.1	51			
57107	Depth drill, long S/SC/SCX 4.1	51			
57108	Depth drill, short S/SC/SCX 4.5	51			
57109	Depth drill, long S/SC/SCX 4.5	51			
57110	Depth drill, short S/SC/SCX 5.5	51			
57116	Sub-Tec <sup>Plus</sup> titanium abutment, GH 1–2, S/RI 3.25–3.75	96			
57117	Sub-Tec <sup>Plus</sup> titanium abutment, GH 2.5–4, S/RI 3.25–3.75	96			
57120	Sub-Tec <sup>Plus</sup> titanium abutment, GH 1–2, S/RI 4.1	96			
57121	Sub-Tec <sup>Plus</sup> titanium abutment, GH 2.5–4, S/RI 4.1	96			
57124	Sub-Tec <sup>Plus</sup> titanium abutment, GH 1–2, S/RI 4.5	96			
57125	Sub-Tec <sup>Plus</sup> titanium abutment, GH 2.5–4, S/RI 4.5	96			
57128	Sub-Tec <sup>Plus</sup> titanium abutment, GH 1–2, S/RI 5.5	96			
57129	Sub-Tec <sup>Plus</sup> titanium abutment, GH 2.5–4, S/RI 5.5	96			
57130	BEGO Guide DS (drill sleeves)	48			
57132	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° GH 1–2, S/RI 3.25–3.75	97			

## INDEX · PRODUCTS BY ARTICLE NUMBERS

REF	Article	Page	REF	Article	Page
57290	Sub-Tec CAD/CAM titanium adhesive abutment no Hex, S/RI 4.5	92	57413	BEGO Guide spoon, Ø2.8 (A3), S/SC/SCX 3.25	42
57291	Sub-Tec CAD/CAM titanium adhesive abutment, S/RI 5.5	92	57414	BEGO Guide spoon, Ø3.25 (A4), S/SC/SCX 3.75	42
57292	Sub-Tec CAD/CAM titanium adhesive abutment no Hex, S/RI 5.5	92	57415	BEGO Guide spoon, Ø1.6 (B1), S/SC/SCX	42
57300	Sub-Tec provisional titanium abutment no Hex, S/RI 3.25–3.75	95	57416	BEGO Guide spoon, Ø2.5 (B2), S/SC/SCX	42
57301	Sub-Tec provisional titanium abutment no Hex, S/RI 4.1	95	57417	BEGO Guide spoon, Ø2.8 (B3), S/SC/SCX 3.25	42
57302	Sub-Tec provisional titanium abutment no Hex, S/RI 4.5	95	57418	BEGO Guide spoon, Ø3.25 (B4), S/SC/SCX 3.75	42
57303	Sub-Tec provisional titanium abutment no Hex, S/RI 5.5	95	57419	BEGO Guide spoon, Ø3.65 (B5), S/SC/SCX 4.1	42
57304	Sub-Tec provisional titanium abutment, S/RI 3.25–3.75	95	57420	BEGO Guide spoon, Ø4.0 (B6), S/SC/SCX 4.5	42
57305	Sub-Tec provisional titanium abutment, S/RI 4.1	95	57421	BEGO Guide tissue punches, Ø4.2 (A), S/SC/SCX/RS/RSX 3.0–3.75	42, 45
57306	Sub-Tec provisional titanium abutment, S/RI 4.5	95	57422	BEGO Guide tissue punches, Ø4.7 (B), S/SC/SCX/RS/RSX 4.1–4.5	42, 45
57307	Sub-Tec provisional titanium abutment, S/RI 5.5	95	57423	BEGO Guide pilot drill, Ø1.6 L18 (X1), S/SC/SCX	43
57308	Pilot marker, short, S/SC/SCX	50	57424	BEGO Guide pilot drill, Ø1.6 L23.5 (Y1), S/SC/SCX	43
57309	Pilot marker, long, S/SC/SCX	50	57425	BEGO Guide pilot drill, Ø1.6 L29 (Z1), S/SC/SCX	43
57324	Healing abutment, conical, S/RI 3.25–3.75	40	57426	BEGO Guide depth drill Ø2.5, L18 (X2), S/SC/SCX	43
57332	Thread tap, S/SC/SCX 3.25	51	57427	BEGO Guide depth drill, Ø2.5 L23.5 (Y2), S/SC/SCX	43
57333	Screw tap, S/SC/SCX 3.75	51	57428	BEGO Guide depth drill Ø2.5, L29 (Z2), S/SC/SCX	43
57334	Screw tap, S/SC/SCX 4.1	51	57429	BEGO Guide depth drill Ø2.8, L18 (X3), S/SC/SCX 3.25	43
57335	Thread tap, S/SC/SCX 4.5	51	57430	BEGO Guide depth drill Ø2.8 L23.5 (Y3), S/SC/SCX 3.25	43
57336	Screw tap, S/SC/SCX 5.5	51	57431	BEGO Guide depth drill Ø2.8, L29 (Z3), S/SC/SCX 3.25	43
57340	BEGO Semados® tray <sup>Plus</sup> , S/SC/SCX 3.25–5.5	50	57432	BEGO Guide depth drill Ø3.25, L18 (X4), S/SC/SCX 3.75	43
57345	Drill stop Tray <sup>Plus</sup> , S/SC/SCX	52	57433	BEGO Guide Pilot Ø3.25 L23.5 (Y4), S/SC/SCX 3.75	43
57347	Drill module, S/SC/SCX 5.5	50	57434	BEGO Guide depth drill Ø3.25, L29 (Z4), S/SC/SCX 3.75	43
57350	Countersink, S/SC/SCX 3.25	51	57435	BEGO Guide depth drill Ø3.65, L18 (X5), S/SC/SCX 4.1	43
57351	Countersink, S/SC/SCX 3.75	51			
57352	Countersink, S/SC/SCX 4.1	51			
57353	Countersink, S/SC/SCX 4.5	51			
57354	Countersink, S/SC/SCX 5.5	51			
57395	BEGO Guide master sleeves, Ø4.2 (A), S/SC/SCX/RS/RSX	42, 45			
57397	BEGO Guide master sleeves, Ø4.7 (B), S/SC/SCX/RS/RSX	42, 45			
57399	BEGO Guide Tray, S/SC/SCX 3.25–4.5	42			
57400	BEGO Guide – pilot drill, short	48			
57401	BEGO Guide – pilot drill, long	48			
57411	BEGO Guide spoon, Ø1.6 (A1), S/SC/SCX	42			
57412	BEGO Guide spoon, Ø2.5 (A2), S/SC/SCX	42			

**Note:** Manufacturer notes about trade names, see page 111.

## INDEX · PRODUCTS BY ARTICLE NUMBERS

REF	Article	Page	REF	Article	Page
57436	BEGO Guide Pilot Ø3.65 L23.5 (Y5), S/SC/SCX 4.1	43	57477	Drill stops, RS/RSX 3.0	55
57437	BEGO Guide depth drill Ø3.65, L29 (Z5), S/SC/SCX 4.1	43	57478	Drill stops, RS/RSX 3.75	55
57438	BEGO Guide depth drill Ø4.0, L18 (X6), S/SC/SCX 4.5	43	57479	Drill stops, RS/RSX 4.1–4.5	55
57439	BEGO Guide Pilot Ø4.0 L23.5 (Y6), S/SC/SCX 4.5	43	57480	Drill stops, RS/RSX 5.5	55
57441	BEGO Guide depth drill Ø4.0, L29 (Z6), S/SC/SCX 4.5	43	57481	Pilot marker, short, RS/RSX	53
57442	BEGO Guide countersink, (3), S/SC/SCX 3.25	43	57482	Pilot marker, long, RS/RSX	53
57443	BEGO Guide Countersink, (4), S/SC/SCX 3.75	43	57483	Drill stop Tray <sup>Plus</sup> , RS/RSX	55
57444	BEGO Guide Countersink, (5), S/SC/SCX 4.1	43	57484	DD D1, RS/RSX 3.0 (depth drill)	54
57445	BEGO Guide Countersink, (6), S/SC/SCX 4.5	43	57485	DD D1, RS/RSX 3.75 (depth drill)	54
57446	BEGO Guide thread tap, (3), S/SC/SCX 3.25	44	57486	DD D1, RS/RSX 4.1 (depth drill)	54
57447	BEGO Guide screw tap, (4), S/SC/SCX 3.75	44	57487	DD D1, RS/RSX 4.5 (depth drill)	54
57448	BEGO Guide screw tap, (5), S/SC/SCX 4.1	44	57488	DD D1, RS/RSX 5.5 (depth drill)	54
57449	BEGO Guide thread tap, (6), S/SC/SCX 4.5	44	57494	Sub-Tec provisional PEEK abutment, S/RI 3.25–3.75	95
57450	BEGO Guide spoon, Ø4.2 (AX), S/SC/SCX	44	57495	Sub-Tec provisional PEEK abutment, S/RI 4.1–4.5	95
57451	BEGO Guide spoon, Ø4.2 (AY), S/SC/SCX	44	57500	BEGO Semados® implant, S 3.25 L8.5	38
57452	BEGO Guide spoon, Ø4.2 (AZ), S/SC/SCX	44	57501	BEGO Semados® implant, S 3.25 L10	38
57453	BEGO Guide spoon, Ø4.7 (BX), S/SC/SCX	44	57502	BEGO Semados® implant, S 3.25 L11.5	38
57454	BEGO Guide spoon, Ø4.7 (BY), S/SC/SCX	44	57503	BEGO Semados® implant, S 3.25 L13	38
57455	BEGO Guide spoon, Ø4.7 (BZ), S/SC/SCX	44	57505	Sub-Tec Multi <sup>Plus</sup> abutment 0°, GH 1, S/RI 3.25–3.75	100
57456	BEGO Guide depth stop ring connector, Ø4.2 (A), S/SC/SCX/RS/RSX	44, 47	57506	Sub-Tec Multi <sup>Plus</sup> abutment 0°, GH 1, S/RI 4.1	100
57457	BEGO Guide depth stop ring connector, Ø4.7 (B), S/SC/SCX/RS/RSX	44, 47	57507	Sub-Tec Multi <sup>Plus</sup> abutment 0°, GH 1, S/RI 4.5	100
57458	BEGO Guide ratchet adapter for connector, S/SC/SCX	44	57508	Sub-Tec Multi <sup>Plus</sup> abutment 0°, GH 3, S/RI 3.25–3.75	100
57459	BEGO Guide center drill, Ø4.2 (A), S/SC/SCX/RS/RSX 3.0–3.75	43, 46	57509	Sub-Tec Multi <sup>Plus</sup> abutment 0°, GH 3, S/RI 4.1	100
57463	BEGO Guide center drill, Ø4.7 (B), S/SC/SCX/RS/RSX 4.1–4.5	43, 46	57510	Sub-Tec Multi <sup>Plus</sup> abutment 0°, GH 3, S/RI 4.5	100
57465	TJU (training jaw) for maxilla	111	57511	Sub-Tec Multi <sup>Plus</sup> abutment 20°, GH 2.3–0.6, S/RI 3.25–3.75	101
57464	TJL (training jaw) for mandible	111	57512	Sub-Tec Multi <sup>Plus</sup> abutment 20°, GH 2.3–0.6, S/RI 4.1	101
57476	Drill stops for depth drill 2.5 RS/RSX	55	57513	Sub-Tec Multi <sup>Plus</sup> abutment 20°, GH 2.3–0.6, S/RI 4.5	101
			57514	Sub-Tec Multi <sup>Plus</sup> abutment 20°, GH 4.0–2.3, S/RI 3.25–3.75	101
			57515	Sub-Tec Multi <sup>Plus</sup> abutment 20°, GH 4.0–2.3, S/RI 4.1	101
			57516	Sub-Tec Multi <sup>Plus</sup> abutment 20°, GH 4.0–2.3, S/RI 4.5	101
			57517	Sub-Tec Multi <sup>Plus</sup> abutment 30°, GH 4.0–1.5, S/RI 3.25–3.75	101
			57518	Sub-Tec Multi <sup>Plus</sup> abutment 30°, GH 4.0–1.5, S/RI 4.1	101

## INDEX · PRODUCTS BY ARTICLE NUMBERS

REF	Article	Page	REF	Article	Page
57519	Sub-Tec Multi <sup>Plus</sup> abutment 30°, GH 4.0-1.5, S/RI 4.5	101	57618	Threadformer, RI 5.5	57
57520	Multi <sup>Plus</sup> healing post	83, 101	57619	Thread tap, RI 3.75	57
57521	Multi <sup>Plus</sup> healing post, Mushroom	83, 101	57620	Screw tap, RI 4.1	57
57522	Multi <sup>Plus</sup> closed-tray impression, short	84, 102	57621	Screw tap, RI 4.5	57
57523	Multi <sup>Plus</sup> open-tray impression	84, 102	57622	Thread tap, RI 5.5	57
57524	Multi <sup>Plus</sup> implant analog, 1 unit	84, 102	57631	Sub-Tec ball attachment, GH 0, S/RI 3.25–3.75	106
57525	Multi <sup>Plus</sup> implant analog, 4 units	84, 102	57632	Sub-Tec ball attachment, GH 0, S/RI 4.1–4.5	106
57526	Multi <sup>Plus</sup> titanium abutment	85, 103	57633	Sub-Tec ball attachment, GH 3, S/RI 3.25–3.75	106
57530	Multi <sup>Plus</sup> alignment aid, 20°	82, 100	57634	Sub-Tec ball attachment, GH 3, S/RI 4.1–4.5	106
57531	Multi <sup>Plus</sup> alignment aid, 30°	82, 100	57635	Sub-Tec ball attachment, GH 5, S/RI 3.25–3.75	106
57532	Multi <sup>Plus</sup> insertion splint	82, 100	57636	Sub-Tec ball attachment, GH 5, S/RI 4.1–4.5	106
57533	Insertion instrument Multi <sup>Plus</sup> abutment 0°, with ratchet connection	82, 100	57656	Sub-Tec CAD/CAM TiBase L, S/RI 3.25–3.75	93
57534	Secondary screw Multi <sup>Plus</sup> (M1.4)	89, 107	57657	Sub-Tec CAD/CAM TiBase L, S/RI 4.1	93
57535	Secondary screw Multi <sup>Plus</sup> (M1.8)	89, 107	57658	Sub-Tec CAD/CAM TiBase L, S/RI 4.5	93
57538	Multi <sup>Plus</sup> Universal	85, 103	57659	Sub-Tec CAD/CAM TiBase L, S/RI 5.5	93
57539	External reamer Multi <sup>Plus</sup>	85, 103	57686	BEGO Guide Sp, Ø2.0 (A1), RS/RSX (reduction sleeve)	45
57540	Internal reamer Multi <sup>Plus</sup>	85, 103	57687	BEGO Guide Sp, Ø2.5 (A2), RS/RSX (reduction sleeve)	45
57554	Multi <sup>Plus</sup> closed-tray impression, long	84, 102	57688	BEGO Guide Sp, Ø2.8 (A3), RS/RSX 3.0 (reduction sleeve)	45
57581	Pilot marker, short, RI	56	57689	BEGO Guide Sp, Ø3.4 (A4), RS/RSX 3.75 (reduction sleeve)	45
57582	Pilot marker, long, RI	56	57690	BEGO Guide Sp, Ø2.0 (B1), RS/RSX (reduction sleeve)	45
57583	Depth drill 3.2, short RI	56	57691	BEGO Guide Sp, Ø2.5 (B2), RS/RSX (reduction sleeve)	45
57584	Depth drill 3.2, long RI	56	57692	BEGO Guide Sp, Ø2.8 (B3), RS/RSX 3.0 (reduction sleeve)	45
57585	Depth drill, short RI 3.75	57	57693	BEGO Guide Sp, Ø3.4 (B4), RS/RSX 3.75 (reduction sleeve)	45
57586	Depth drill, long RI 3.75	57	57694	BEGO Guide Sp, Ø3.8 (B5), RS/RSX 4.1 (reduction sleeve)	45
57587	Depth drill, short RI 4.1	57	57695	BEGO Guide Sp, Ø4.1 (B6), RS/RSX 4.5 (reduction sleeve)	45
57588	Depth drill, long RI 4.1	57	57696	BEGO Guide PD, Ø2.0 L18 (X1), RS/RSX (pilot drill)	46
57589	Depth drill, short RI 4.5	57	57697	BEGO Guide pilot drill, Ø2.0 L23.5 (Y1), RS/RSX (pilot drill)	46
57590	Depth drill, long RI 4.5	57	57698	BEGO Guide PD, Ø2.0 L29 (Z1), RS/RSX (pilot drill)	46
57591	Depth drill, short RI 5.5	57	57699	BEGO Semados® RSX demo implants 3.0	111
57592	Countersink, RI 3.75	57	57700	BEGO Semados® implant, S 4.5 L7	38
57593	Countersink, RI 4.1	57	57701	BEGO Semados® implant, S 4.5 L8.5	38
57594	Countersink, RI 4.5	57	57702	BEGO Semados® implant, S 4.5 L10	38
57595	Countersink, RI 5.5	57			
57598	Paralleling post, RI	58			
57601	BEGO Semados® implant, S 3.75 L8.5	38			
57602	BEGO Semados® implant, S 3.75 L10	38			
57603	BEGO Semados® implant, S 3.75 L11.5	38			
57604	BEGO Semados® implant, S 3.75 L13	38			
57612	BEGO Semados® Tray <sup>Plus</sup> , RI 3.75–5.5	56			
57613	Drill module, RI 5.5	56			
57615	Threadformer, RI 3.75	57			
57616	Threadformer, RI 4.1	57			
57617	Threadformer, RI 4.5	57			

**Note:** Manufacturer notes about trade names, see page 111.

## INDEX · PRODUCTS BY ARTICLE NUMBERS

REF	Article	Page	REF	Article	Page
57703	BEGO Semados® implant, S 4.5 L11.5	38	57739	BEGO Semados® implant, RI 5.5 L10	32
57704	BEGO Semados® implant, S 4.5 L13	38	57740	BEGO Semados® implant, RI 5.5 L11.5	32
57708	BEGO Semados® implant, RI 3.75 L8.5	32	57741	BEGO Semados® implant, RI 5.5 L13	32
57709	BEGO Semados® implant, RI 3.75 L10	32	57743	Sub-Tec Easy-Con abutment, L1, S/RI 3.75–4.1	104
57710	BEGO Semados® implant, RI 3.75 L11.5	32	57744	Sub-Tec Easy-Con abutment, L2, S/RI 3.75–4.1	104
57711	BEGO Semados® implant, RI 3.75 L13	32	57745	Sub-Tec Easy-Con abutment, L3, S/RI 3.75–4.1	104
57713	BEGO Guide PD, Ø2.5 L18 (X2), RS/RSX (depth drill)	46	57746	Sub-Tec Easy-Con abutment, L4, S/RI 3.75–4.1	104
57714	BEGO Guide pilot drill, Ø2.5 L23.5 (Y2), RS/RSX (depth drill)	46	57747	Sub-Tec Easy-Con abutment, L1, S/RI 4.5	104
57715	BEGO Guide PD, Ø2.5 L29 (Z2), RS/RSX (depth drill)	46	57748	Sub-Tec Easy-Con abutment, L2, S/RI 4.5	104
57716	BEGO Guide DD, Ø2.8 L18 (X3), RS/RSX 3.0 (depth drill)	46	57749	Sub-Tec Easy-Con abutment, L3, S/RI 4.5	104
57717	BEGO Guide DD, Ø2.8 L23.5 (Y3), RS/RSX 3.0 (depth drill)	46	57750	Sub-Tec Easy-Con abutment, L4, S/RI 4.5	104
57718	BEGO Semados® implant, RI 4.1 L8.5	32	57751	Easy-Con impression coping	86, 104
57719	BEGO Semados® implant, RI 4.1 L10	32	57752	Easy-Con laboratory set	87, 105
57720	BEGO Semados® implant, RI 4.1 L11.5	32	57753	Easy-Con instrument	87, 105
57721	BEGO Semados® implant, RI 4.1 L13	32	57754	Easy-Con production insert (black)	87, 105
57723	BEGO Guide DD, Ø2.8 L29 (Z3), RS/RSX 3.0 (depth drill)	46	57755	Easy-Con retention insert (blue)	87, 105
57724	BEGO Guide DD, Ø3.4 L18 (X4), RS/RSX 3.75 (depth drill)	46	57756	Easy-Con retention insert (pink)	87, 105
57725	BEGO Guide DD, Ø3.4 L23.5 (Y4), RS/RSX 3.75 (depth drill)	46	57757	Easy-Con retention insert (transparent)	87, 105
57726	BEGO Guide DD, Ø3.4 L29 (Z4), RS/RSX 3.75 (depth drill)	46	57758	Easy-Con retention insert (red)	87, 105
57727	BEGO Guide DD, Ø3.8 L18 (X5), RS/RSX 4.1 (depth drill)	46	57759	Easy-Con retention insert (green)	87, 105
57728	BEGO Semados® implant, RI 4.5 L8.5	32	57760	Easy-Con analog	86, 104
57729	BEGO Semados® implant, RI 4.5 L10	32	57764	PS HP, Ø3.0 L3, RS/RSX 3.0 (healing abutment)	34
57730	BEGO Semados® implant, RI 4.5 L11.5	32	57765	PS HP, Ø3.0 L5, RS/RSX 3.0 (healing abutment)	34
57731	BEGO Semados® implant, RI 4.5 L13	32	57766	PS HP, Ø3.0 L7, RS/RSX 3.0 (healing abutment)	34
57733	BEGO Guide DD, Ø3.8 L23.5 (Y5), RS/RSX 4.1 (depth drill)	46	57767	PS HP, Ø4.0 L3, RS/RSX 3.0 (healing abutment)	34
57734	BEGO Guide DD, Ø3.8 L29 (Z5), RS/RSX 4.1 (depth drill)	46	57768	PS HP, Ø4.0 L5, RS/RSX 3.0 (healing abutment)	34
57735	BEGO Guide DD, Ø4.1 L18 (X6), RS/RSX 4.5 (depth drill)	46	57769	PS HP, Ø4.0 L7, RS/RSX 3.0 (healing abutment)	34
57736	BEGO Guide DD, Ø4.1 L23.5 (Y6), RS/RSX 4.5 (depth drill)	46	57773	PS CTI, RS/RSX 3.0 (impression set, closed)	75
57737	BEGO Guide DD, Ø4.1 L29 (Z6), RS/RSX 4.5 (depth drill)	46	57774	PS CTI, RS/RSX 3.0 (impression set, open)	75
57738	BEGO Semados® implant, RI 5.5 L8.5	32	57776	PS TiA, GH 2.5–4, RS/RSX 3.0 (solid abutment)	76
			57778	PS ITA, RS/RSX 3.0 (temporary abutment)	76
			57781	PS TiB, RS/RSX 3.0 (adhesive abutment)	72
			57782	Pscrew (prosthesis screw Ø3.0)	89
			57784	Pscrew (prosthesis screw, for CAD positioner Ø3.0)	89
			57796	PS IMPA, RS/RSX 3.0 (implant analog)	75
			57797	PS TiAA, 15° P GH 2.5–4, RS/RSX 3.0 (solid abutment)	76
			57798	PS TiAA, 15° E GH 2.5–4, RS/RSX 3.0 (solid abutment)	76
			57799	PS CTI, SC/SCX/RS/RSX/RI*1 3.75 (impression set, closed)	75
			57800	PS CTI, SC/SCX/RS/RSX/RI*1 4.1 (impression set, closed)	75

## INDEX · PRODUCTS BY ARTICLE NUMBERS

REF	Article	Page	REF	Article	Page
57801	PS CTI, SC/SCX/RS/RSX/RI*1 4.5 (impression set, closed)	75	57823	PS TiB, GH 0, SC/SCX/RS/RSX/RI*1 3.25–3.75 (adhesive abutment)	73
57802	PS CTI, SC/SCX/RS/RSX/RI*1 5.5 (impression set, closed)	75	57824	PS TiB, GH 0, SC/SCX/RS/RSX/RI*1 4.1 (adhesive abutment)	73
57803	PS OTI, SC/SCX/RS/RSX/RI*1 3.75 (impression set, open)	75	57825	PS TiB, GH 0, SC/SCX/RS/RSX/RI*1 4.5 (adhesive abutment)	73
57804	PS OTI, SC/SCX/RS/RSX/RI*1 4.1 (impression set, open)	75	57826	PS TiB, GH 0, SC/SCX/RS/RSX/RI*1 5.5 (adhesive abutment)	73
57805	PS OTI, SC/SCX/RS/RSX/RI*1 4.5 (impression set, open)	75	57827	PS TiB NH, GH 0, SC/SCX/RS/RSX/RI*1 3.25–3.75 (adhesive abutment no Hex)	74
57806	PS OTI, SC/SCX/RS/RSX/RI*1 5.5 (impression set, open)	75	57828	PS TiB NH, GH 0, SC/SCX/RS/RSX/RI*1 4.1 (adhesive abutment no Hex)	74
57807	PS HP, Ø 4.5 L3, SC/SCX/RS/RSX/RI*1 3.25–3.75 (healing abutment)	34	57829	PS TiB NH, GH 0, SC/SCX/RS/RSX/RI*1 4.5 (adhesive abutment no Hex)	74
57808	PS HP, Ø 4.5 L5, SC/SCX/RS/RSX/RI*1 3.25–3.75 (healing abutment)	34	57830	PS TiB NH, GH 0, SC/SCX/RS/RSX/RI*1 5.5 (adhesive abutment no Hex)	74
57809	PS HP, Ø 5.0 L3, SC/SCX/RS/RSX/RI*1 4.1 (healing abutment)	34	57831	PS UNI, SC/SCX/RS/RSX/RI*1 3.25–3.75 (Universal abutment)	80
57810	PS HP, Ø 5.0 L5, SC/SCX/RS/RSX/RI*1 4.1 (healing abutment)	34	57832	PS UNI, SC/SCX/RS/RSX/RI*1 4.1 (Universal abutment)	80
57811	PS HP, Ø 5.5 L3, SC/SCX/RS/RSX/RI*1 4.5 (healing abutment)	34	57833	PS UNI, SC/SCX/RS/RSX/RI*1 4.5 (Universal abutment)	80
57812	PS HP, Ø 5.5 L5, SC/SCX/RS/RSX/RI*1 4.5 (healing abutment)	34	57834	PS UNI, SC/SCX/RS/RSX/RI*1 5.5 (Universal abutment)	80
57813	PS HP, Ø 6.5 L3, SC/SCX/RS/RSX/RI*1 5.5 (healing abutment)	34	57835	PS UNI NH, SC/SCX/RS/RSX/RI*1 3.25– 3.75 (Universal no Hex abutment)	80
57814	PS HP, Ø 6.5 L5, SC/SCX/RS/RSX/RI*1 5.5 (healing abutment)	34	57836	PS UNI NH, SC/SCX/RS/RSX/RI*1 4.1 (Universal abutment no Hex)	80
57815	PS HPW, Ø 5.5 L3, SC/SCX/RS/RSX/RI*1 3.25–3.75 (healing abutment)	35	57837	PS UNI NH, SC/SCX/RS/RSX/RI*1 4.5 (Universal abutment no Hex)	80
57816	PS HPW, Ø 6.0 L3, SC/SCX/RS/RSX/RI*1 4.1 (healing abutment)	35	57838	PS UNI NH, SC/SCX/RS/RSX/RI*1 5.5 (Universal abutment no Hex)	80
57817	PS HPW, Ø 6.5 L3, SC/SCX/RS/RSX/RI*1 4.5 (healing abutment)	35	57840	BEGO Semados® implant, S 4.1 L7	38
57818	PS HPW, Ø 7.0 L3, SC/SCX/RS/RSX/RI*1 5.5 (healing abutment)	35	57841	BEGO Semados® implant, S 4.1 L8.5	38
57819	PS IMPA, SC/SCX/RS/RSX/RI*1 3.75 (implant analog)	75	57842	BEGO Semados® implant, S 4.1 L10	38
57820	PS IMPA, SC/SCX/RS/RSX/RI*1 4.1 (implant analog)	75	57843	BEGO Semados® implant, S 4.1 L11.5	38
57821	PS IMPA, SC/SCX/RS/RSX/RI*1 4.5 (implant analog)	75	57844	BEGO Semados® implant, S 4.1 L13	38
57822	PS IMPA, SC/SCX/RS/RSX/RI*1 5.5 (implant analog)	75	57846	PS TiA, GH 1–2, SC/SCX/RS/RSX/RI*1 3.25–3.75 (solid abutment)	78
			57847	PS TiA, GH 2.5–4, SC/SCX/RS/RSX/RI*1 3.25–3.75 (solid abutment)	78
			57848	PS TiA, GH 1–2, SC/SCX/RS/RSX/RI*1 4.1 (solid abutment)	78
			57849	PS TiA, GH 2.5–4, SC/SCX/RS/RSX/RI*1 4.1 (solid abutment)	78

**Note:** Manufacturer notes about trade names, see page 111.

\*1 Version of the BEGO Semados® RI implants, with Platform Switch design

## INDEX · PRODUCTS BY ARTICLE NUMBERS

REF	Article	Page	REF	Article	Page
57850	PS TiA, GH 1–2, SC/SCX/RS/RSX/RI*1 4.5 (solid abutment)	78	57897	PS TiAA, 15° P GH 1–2, SC/SCX/RS/RSX/RI*1 4.5 (solid abutment)	79
57851	PS TiA, GH 2.5–4, SC/SCX/RS/RSX/RI*1 4.5 (solid abutment)	78	57898	PS TiAA, 15° P GH 2.5–4, SC/SCX/RS/RSX/RI*1 4.5 (solid abutment)	79
57852	PS TiA, GH 1–2, SC/SCX/RS/RSX/RI*1 5.5 (solid abutment)	78	57899	PS TiAA, 15° E GH 1–2, SC/SCX/RS/RSX/RI*1 4.5 (solid abutment)	79
57853	PS TiA, GH 2.5–4, SC/SCX/RS/RSX/RI*1 5.5 (solid abutment)	78	57900	PS TiAA, 15° E GH 2.5–4, SC/SCX/RS/RSX/RI*1 4.5 (solid abutment)	79
57854	PS TTiA, SC/SCX/RS/RSX/RI*1 3.25–3.75 (temporary abutment)	77	57901	BEGO Semados® implant, S 5.5 L8.5	38
57855	PS TTiA, SC/SCX/RS/RSX/RI*1 4.1 (temporary abutment)	77	57902	BEGO Semados® implant, S 5.5 L10	38
57856	PS TTiA, SC/SCX/RS/RSX/RI*1 4.5 (provisional abutment)	77	57903	BEGO Semados® implant, S 5.5 L11.5	38
57857	PS TTiA, SC/SCX/RS/RSX/RI*1 5.5 (temporary abutment)	77	57904	BEGO Semados® implant, S 5.5 L13	38
57858	PS TTiA NH, SC/SCX/RS/RSX/RI*1 3.25– 3.75 (temporary abutment no Hex)	77	57905	PS TiAA, 15° P GH 1–2, SC/SCX/RS/RSX/RI*1 5.5 (solid abutment)	79
57859	PS TTiA NH, SC/SCX/RS/RSX/RI*1 4.1 (temporary abutment no Hex)	77	57906	PS TiAA, 15° P GH 2.5–4, SC/SCX/RS/RSX/RI*1 5.5 (solid abutment)	79
57860	PS TTiA NH, SC/SCX/RS/RSX/RI*1 4.5 (provisional abutment no Hex)	77	57907	PS TiAA, 15° E GH 1–2, SC/SCX/RS/RSX/RI*1 5.5 (solid abutment)	79
57861	PS TTiA NH, SC/SCX/RS/RSX/RI*1 5.5 (temporary abutment no Hex)	77	57908	PS TiAA, 15° E GH 2.5–4, SC/SCX/RS/RSX/RI*1 5.5 (solid abutment)	79
57862	BEGO Semados® implant, RSX 3.0 L10	29	57909	PS TiAA, 20° P GH 1–2, SC/SCX/RS/RSX/RI*1 3.25–3.75 (solid abutment)	79
57863	BEGO Semados® implant, RSX 3.0 L11.5	29	57910	PS TiAA, 20° P GH 2.5–4, SC/SCX/RS/RSX/RI*1 3.25–3.75 (solid abutment)	79
57864	BEGO Semados® implant, RSX 3.0 L13	29	57911	PS TiAA, 20° E GH 1–2, SC/SCX/RS/RSX/RI*1 3.25–3.75 (solid abutment)	79
57889	PS TiAA, 15° P GH 1–2, SC/SCX/RS/RSX/RI*1 3.25–3.75 (solid abutment)	79	57912	PS TiAA, 20° E GH 2.5–4, SC/SCX/RS/RSX/RI*1 3.25–3.75 (solid abutment)	79
57890	PS TiAA, 15° P GH 2.5–4, SC/SCX/RS/RSX/RI*1 3.25–3.75 (solid abutment)	79	57913	PS TiAA, 20° P GH 1–2, SC/SCX/RS/RSX/RI*1 4.1 (solid abutment)	79
57891	PS TiAA, 15° E GH 1–2, SC/SCX/RS/RSX/RI*1 3.25–3.75 (solid abutment)	79	57914	PS TiAA, 20° P GH 2.5–4, SC/SCX/S/RSX/RI*1 4.1 (solid abutment)	79
57892	PS TiAA, 15° E GH 2.5–4, SC/SCX/RS/RSX/RI*1 3.25–3.75 (solid abutment)	79	57915	PS TiAA, 20° E GH 1–2, SC/SCX/RS/RSX/RI*1 4.1 (solid abutment)	79
57893	PS TiAA, 15° P GH 1–2, SC/SCX/RS/RSX/RI*1 4.1 (solid abutment)	79	57916	PS TiAA, 20° E GH 2.5–4, SC/SCX/RS/RSX/RI*1 4.1 (solid abutment)	79
57894	PS TiAA, 15° P GH 2.5–4, SC/SCX/RS/RSX/RI*1 4.1 (solid abutment)	79	57917	PS TiAA, 20° P GH 1–2, SC/SCX/RS/RSX/RI*1 4.5 (solid abutment)	79
57895	PS TiAA, 15° E GH 1–2, SC/SCX/RS/RSX/RI*1 4.1 (solid abutment)	79	57918	PS TiAA, 20° P GH 2.5–4, SC/SCX/RS/RSX/RI*1 4.5 (solid abutment)	79
57896	PS TiAA, 15° E GH 2.5–4, SC/SCX/RS/RSX/RI*1 4.1 (solid abutment)	79			

## INDEX · PRODUCTS BY ARTICLE NUMBERS

REF	Article	Page	REF	Article	Page
57919	PS TIAA, 20° E GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	79	57954	Implant cover screw, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5	34
57920	PS TIAA, 20° E GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	79	57955	Depth gauge, RS/RSX	59
57921	PS TIAA, 20° P GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	79	57956	Paralleling post, RS/RSX	58
57922	PS TIAA, 20° P GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	79	57959	Radiographic template, RS/RSX implants	20
57923	PS TIAA, 20° E GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	79	57962	BEGO Semados® implant, RS 3.0 L10	28
57924	PS TIAA, 20° E GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	79	57963	BEGO Semados® implant, RS 3.0 L11.5	28
57926	Depth drill 2.5 short, RS/RSX	57	57964	BEGO Semados® implant, RS 3.0 L13	28
57927	Depth drill 2.5 long, RS/RSX	53	57993	PS UNI PScrew (prosthesis screw)	89
57928	Depth drill short, RS/RSX 3.0	54	58051	BEGO Guide CS, (3), RS/RSX 3.0 (countersink)	46
57929	Depth drill long, RS/RSX 3.0	54	58052	BEGO Guide System (4) RS/RSX 3.75 (countersink)	46
57930	Depth drill short, RS/RSX 3.75	54	58053	BEGO Guide System (5) RS/RSX 4.1 (countersink)	46
57931	Depth drill long, RS/RSX 3.75	54	58054	BEGO Guide System (6) RS/RSX 4.5 (countersink)	46
57932	Depth drill short, RS/RSX 4.1	54	58055	BEGO Guide ST, (3), RS/RSX 3.0 (thread tap)	47
57933	Depth drill long, RS/RSX 4.1	54	58056	BEGO Guide ST, (4), RS/RSX 3.75 (thread tap)	47
57934	Depth drill short, RS/RSX 4.5	54	58057	BEGO Guide ST, (5), RS/RSX 4.1 (thread tap)	47
57935	Depth drill long, RS/RSX 4.5	54	58058	BEGO Guide ST (6) RS/RSX 4.5 (thread tap)	47
57936	Depth drill short, RS/RSX 5.5	54	58059	BEGO Guide Conn, with contra-angle connection, Ø 4.2 (AX), RS/RSX (connector)	47
57937	Countersink, RS/RSX 3.0	54	58060	BEGO Guide Conn, with contra-angle connection, Ø 4.2 (AY), RS/RSX (connector)	47
57938	Countersink, RS/RSX 3.75	54	58061	BEGO Guide Conn, with contra-angle connection, Ø 4.2 (AZ), RS/RSX (connector)	47
57939	Countersink, RS/RSX 4.1	54	58062	BEGO Guide Conn, with contra-angle connection, Ø 4.7 (BX), RS/RSX (connector)	47
57940	Countersink, RS/RSX 4.5	54	58063	BEGO Guide Conn, with contra-angle connection, Ø 4.7 (BY), RS/RSX (connector)	47
57941	Countersink, RS/RSX 5.5	54	58064	BEGO Guide Conn, with contra-angle connection, Ø 4.7 (BZ), RS/RSX (connector)	47
57943	Thread tap, RS/RSX 3.0	54	58065	BEGO Guide Conn, with ratchet connection, Ø 4.2 (AX), RS/RSX (connector)	47
57944	Thread tap, RS/RSX 3.75	54	58066	BEGO Guide Conn, with ratchet connection, Ø 4.2 (AY), RS/RSX (connector)	47
57945	Screw tap, RS/RSX 4.1	54	58067	BEGO Guide Conn, with ratchet connection, Ø 4.2 (AZ), RS/RSX (connector)	47
57946	Thread tap, RS/RSX 4.5	54	58068	BEGO Guide Conn, with ratchet connection, Ø 4.7 (BX), RS/RSX (connector)	47
57947	Thread tap, RS/RSX 5.5	54			
57948	Drill module, RS/RSX 5.5	53			
57949	BEGO Semados® Tray <sup>Plus</sup> , RS/RSX 3.0–5.5	53			
57950	Implant cover screw, RS/RSX 3.0	34			
57951	Implant cover screw, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.75	34			
57952	Implant cover screw, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1	34			
57953	Implant cover screw, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5	34			

**Note:** Manufacturer notes about trade names, see page 111.

\*<sup>1</sup> Version of the BEGO Semados® RI implants, with Platform Switch design

## INDEX · PRODUCTS BY ARTICLE NUMBERS

REF	Article	Page	REF	Article	Page
58069	BEGO Guide Conn, with ratchet connection, Ø4.7 (BY), RS/RSX (connector)	47	58101	PS Multi <sup>Plus</sup> , 0° GH 3, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (abutment)	82
58070	BEGO Guide Conn, with ratchet connection, Ø4.7 (BZ), RS/RSX (connector)	47	58102	PS Multi <sup>Plus</sup> , 0° GH 1, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (abutment)	82
58071	BEGO Guide Tr, RS/RSX 3.0–4.5 (surgical tray)	45	58103	PS Multi <sup>Plus</sup> , 0° GH 3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (abutment)	82
58072	PS PPA, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (temporary abutment)	77	58104	PS Multi <sup>Plus</sup> , 0° GH 1, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (abutment)	82
58073	PS PPA SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (temporary abutment)	77	58105	PS Multi <sup>Plus</sup> , 0° GH 3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (abutment)	82
58074	PS PPA SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (temporary abutment)	77	58108	PS Multi <sup>Plus</sup> , 20° GH 2.3–0.6, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (abutment)	83
58075	PS PPA SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (temporary abutment)	77	58109	PS Multi <sup>Plus</sup> , 20° GH 4.0–2.3, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (abutment)	83
58076	PS ITA, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (temporary abutment)	77	58110	PS Multi <sup>Plus</sup> , 20° GH 2.3–0.6, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (abutment)	83
58077	PS ITA SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (temporary abutment)	77	58111	PS Multi <sup>Plus</sup> , 20° GH 4.0–2.3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (abutment)	83
58078	PS ITA SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (temporary abutment)	77	58112	PS Multi <sup>Plus</sup> , 20° GH 2.3–0.6, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (abutment)	83
58088	PS TiA, conical, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (solid abutment)	78	58113	PS Multi <sup>Plus</sup> , 20° GH 4.0–2.3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (abutment)	83
58089	PS TiA, conical, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (solid abutment)	78	58116	PS Multi <sup>Plus</sup> , 30° GH 4.0–1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (abutment)	83
58090	PS TiA, conical, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	78	58117	PS Multi <sup>Plus</sup> , 30° GH 4.0–1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (abutment)	83
58091	PS TiA, conical, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	78	58118	PS Multi <sup>Plus</sup> , 30° GH 4.0–1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (abutment)	83
58092	PS GCO, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (gold cast-on abutment)	81	58120	PS BA, GH 0, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (ball attachment abutment)	88
58093	PS GCO SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (gold cast-on abutment)	81	58121	PS BA GH 3, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (ball attachment abutment)	88
58094	PS GCO SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (gold cast-on abutment)	81	58122	PS BA GH 5, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (ball attachment abutment)	88
58096	PS GCO NH, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (gold cast-on abutment no Hex)	81	58123	PS BA, GH 0, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (ball attachment abutment)	88
58097	PS GCO NH, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (gold cast-on abutment no Hex)	81	58124	PS BA GH 3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (ball attachment abutment)	88
58098	PS GCO NH, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (gold cast-on abutment no Hex)	81	58125	PS BA, GH 5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (ball attachment abutment)	88
58099	PS GCO NH, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (gold cast-on abutment no Hex)	81	58126	PS BA, GH 0, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (ball attachment abutment)	88
58100	PS Multi <sup>Plus</sup> , 0° GH 1, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (abutment)	82	58127	PS BA, GH 3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (ball attachment abutment)	88

## INDEX · PRODUCTS BY ARTICLE NUMBERS

REF	Article	Page	REF	Article	Page
58128	PS BA, GH 5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (ball attachment abutment)	88	58160	BEGO Semados® implant, SC 3.25 L8.5	24
58130	PS Easy-Con, L1, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.75 (abutment)	86	58161	BEGO Semados® implant, SC 3.25 L10	24
58131	PS Easy-Con, L2, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.75 (abutment)	86	58162	BEGO Semados® implant, SC 3.25 L11.5	24
58132	PS Easy-Con, L3, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.75 (abutment)	86	58163	BEGO Semados® implant, SC 3.25 L13	24
58133	PS Easy-Con, L4, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.75 (abutment)	86	58164	BEGO Semados® implant, SC 3.25 L15	24
58134	PS Easy-Con, L1, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (abutment)	86	58165	BEGO Semados® implant, SC 3.75 L8.5	24
58135	PS Easy-Con, L2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (abutment)	86	58166	BEGO Semados® implant, SC 3.75 L10	24
58136	PS Easy-Con, L3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (abutment)	86	58167	BEGO Semados® implant, SC 3.75 L11.5	24
58137	PS Easy-Con, L4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (abutment)	86	58168	BEGO Semados® implant, SC 3.75 L13	24
58138	PS Easy-Con, L1, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (abutment)	86	58169	BEGO Semados® implant, SC 3.75 L15	24
58139	PS Easy-Con, L2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (abutment)	86	58170	BEGO Semados® implant, SC 4.1 L7	24
58140	PS Easy-Con, L3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (abutment)	86	58171	BEGO Semados® implant, SC 4.1 L8.5	24
58141	PS Easy-Con, L4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (abutment)	86	58172	BEGO Semados® implant, SC 4.1 L10	24
58142	PS Easy-Con, L2, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (abutment)	86	58173	BEGO Semados® implant, SC 4.1 L11.5	24
58143	PS Easy-Con, L4, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (abutment)	86	58174	BEGO Semados® implant, SC 4.1 L13	24
58146	PS TPA, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (temporary abutment)	77	58175	BEGO Semados® implant, SC 4.1 L15	24
58147	PS TPA SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (temporary abutment)	77	58176	BEGO Semados® implant, SC 4.5 L7	24
58148	PS TPA SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (temporary abutment)	77	58177	BEGO Semados® implant, SC 4.5 L8.5	24
58150	PS HP, Ø4.5 L7, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (healing abutment)	34	58178	BEGO Semados® implant, SC 4.5 L10	24
58151	PS HP, Ø5.0 L7, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (healing abutment)	34	58179	BEGO Semados® implant, SC 4.5 L11.5	24
58152	PS HP, Ø5.5 L7, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (healing abutment)	34	58180	BEGO Semados® implant, SC 4.5 L13	24
58153	PS HP, Ø6.5 L7, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (healing abutment)	34	58181	BEGO Semados® implant, SC 4.5 L15	24
			58182	BEGO Semados® implant, SC 5.5 L7	24
			58183	BEGO Semados® implant, SC 5.5 L8.5	24
			58184	BEGO Semados® implant, SC 5.5 L10	24
			58185	BEGO Semados® implant, SC 5.5 L11.5	24
			58186	BEGO Semados® implant, SC 5.5 L13	24
			58191	CAD SP, S/SC/SCX/RS/RSX/RI 3.25–3.75 (scansupport)	73, 93
			58192	CAD SP, S/SC/SCX/RS/RSX/RI 4.1 (scansupport)	73, 93
			58193	CAD SP, S/SC/SCX/RS/RSX/RI 4.5 (scansupport)	73, 93
			58194	CAD SP, S/SC/SCX/RS/RSX/RI 5.5 (scansupport)	73, 93
			58196*	PS Multi <sup>Plus</sup> , 0° GH 2, SC/SCX/RS/RSX/RI 3.25–3.75 (abutment)	82
			58197*	PS Multi <sup>Plus</sup> , 0° GH 2, SC/SCX/RS/RSX/RI 4.1 (abutment)	82
			58198*	PS Multi <sup>Plus</sup> , 0° GH 2, SC/SCX/RS/RSX/RI 4.5 (abutment)	82
			58199	Insertion instrument Multi <sup>Plus</sup> abutment 0°, with contra-angle connection	82, 92
			58200	PS HPW, Ø5.5 L5, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (healing abutment)	35

**Note:** Manufacturer notes about trade names, see page 111.

\* Planned availability from November 2021

\*<sup>1</sup> Version of the BEGO Semados® RI implants, with Platform Switch design

## INDEX · PRODUCTS BY ARTICLE NUMBERS

REF	Article	Page	REF	Article	Page
58201	PS HPW, Ø 5.5 L7, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (healing abutment)	35	58265	BEGO Semados® implant, SCX 3.75 L8.5	25
58202	PS HPW, Ø 6.0 L5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (healing abutment)	35	58266	BEGO Semados® implant, SCX 3.75 L10	25
58203	PS HPW, Ø 6.0 L7, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (healing abutment)	35	58267	BEGO Semados® implant, SCX 3.75 L11.5	25
58204	PS HPW, Ø 6.5 L5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (healing abutment)	35	58268	BEGO Semados® implant, SCX 3.75 L13	25
58205	PS HPW, Ø 6.5 L7, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (healing abutment)	35	58269	BEGO Semados® implant, SCX 3.75 L15	25
58206	PS HPW, Ø 7.0 L5, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (healing abutment)	35	58270	BEGO Semados® implant, SCX 4.1 L7	25
58216*	PS Multi <sup>Plus</sup> , 0° GH 4, SC/SCX/RS/RSX/RI 3.25–3.75 (abutment)	82	58271	BEGO Semados® implant, SCX 4.1 L8.5	25
58217*	PS Multi <sup>Plus</sup> , 0° GH 4, SC/SCX/RS/RSX/RI 4.1 (abutment)	82	58272	BEGO Semados® implant, SCX 4.1 L10	25
58218*	PS Multi <sup>Plus</sup> , 0° GH 4, SC/SCX/RS/RSX/RI 4.5 (abutment)	82	58273	BEGO Semados® implant, SCX 4.1 L11.5	25
58219	ST PMB, Ø 16, S/RI 3.25–5.5 (milling blank)	93	58274	BEGO Semados® implant, SCX 4.1 L13	25
58221	PS PMB, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–5.5 (TI-Form milling blank)	74	58275	BEGO Semados® implant, SCX 4.1 L15	25
58226	PS PMB, Ø 16, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–5.5 (milling blank)	74	58276	BEGO Semados® implant, SCX 4.5 L7	25
58242	BEGO Semados® SCX implant large-scale model	110	58277	BEGO Semados® implant, SCX 4.5 L8.5	25
58243	Maxilla demonstration model, SCX implants	111	58278	BEGO Semados® implant, SCX 4.5 L10	25
58244	BEGO Semados® SC demo implants	111	58279	BEGO Semados® implant, SCX 4.5 L11.5	25
58245	BEGO Semados® SCX demo implants	111	58280	BEGO Semados® implant, SCX 4.5 L13	25
58246	Radiographic template, SC/SCX implants	20	58281	BEGO Semados® implant, SCX 4.5 L15	25
58247	PS AS (selection set)	78	58282	BEGO Semados® implant, SCX 5.5 L7	25
58250	PS CADP, RS/RSX 3.0 (CAD positioner)	72	58283	BEGO Semados® implant, SCX 5.5 L8.5	25
58251	PS CADP, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (CAD positioner)	73	58284	BEGO Semados® implant, SCX 5.5 L10	25
58252	PS CADP, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (CAD positioner)	73	58285	BEGO Semados® implant, SCX 5.5 L11.5	25
58253	PS CADP, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (CAD positioner)	73	58286	BEGO Semados® implant, SCX 5.5 L13	25
58254	PS CADP, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (CAD positioner)	73	58290	Implant cover screw, SC/SCX 3.25	34
58255	CADP Multi <sup>Plus</sup> (CAD positioner)	85, 103	58315	PS IMPA, SC/SCX 3.25 (implant analog)	80
58260	BEGO Semados® implant, SCX 3.25 L8.5	25	58316	PS CTI, SC/SCX 3.25 (impression set, closed)	75
58261	BEGO Semados® implant, SCX 3.25 L10	25	58317	PS OTI, SC/SCX 3.25 (impression set, open)	75
58262	BEGO Semados® implant, SCX 3.25 L11.5	25	58319	ST PMB, Ø 11.5, S/RI 3.25–5.5 (milling blank)	93
58263	BEGO Semados® implant, SCX 3.25 L13	25	58322	BEGO Semados® RI* <sup>1</sup> implant large-scale model	110
58264	BEGO Semados® implant, SCX 3.25 L15	25	58326	PS PMB, Ø 11.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–5.5(milling blank)	74
			58330	BEGO Semados® implant, S-TG (PS) 3.75 L10	22
			58331	BEGO Semados® implant, S-TG (PS) 3.75 L13	22
			58333	BEGO Semados® implant, S-TG (PS) 4.1 L10	22
			58334	BEGO Semados® implant, S-TG (PS) 4.1 L13	22
			58336*	Sub-Tec Multi <sup>Plus</sup> abutment 0°, GH 2, S/RI 3.25–3.75	100
			58337*	Sub-Tec Multi <sup>Plus</sup> abutment 0°, GH 2, S/RI 4.1	100
			58338*	Sub-Tec Multi <sup>Plus</sup> abutment 0°, GH 2, S/RI 4.5	100
			58345	BEGO Semados® RI* <sup>1</sup> demo implant	111
			58346	BEGO Semados® Starter/Compact Tray <sup>Plus</sup> S/SC/SCX 3.75–4.5	50

## INDEX · PRODUCTS BY ARTICLE NUMBERS

REF	Article	Page	REF	Article	Page
58347	BEGO Semados® Starter/Compact Tray <sup>Plus</sup> (empty) S/SC/SCX 3.75–4.5	50	58489	naturesQue MaxOss P, 0.25–1.0mm 1.0ml	12
58348	BEGO Semados® Starter/Compact Tray <sup>Plus</sup> , RS/RSX 3.75–4.5	53	58490	naturesQue MaxOss P, 0.25–1.0mm 2.0ml	12
58349	BEGO Semados®, Starter/Compact Tray <sup>Plus</sup> (empty), RS/RSX 3.75–4.5	53	58491	naturesQue MaxOss P, 0.25–1.0mm 4.0ml	12
58350	BEGO Semados® Tray <sup>Plus</sup> (empty), RS/RSX 3.0–5.5	53	58492	naturesQue MaxOss P, 1.0–2.0mm 1.0ml	12
58351	BEGO Semados® Tray <sup>Plus</sup> (empty) S/SC/SCX 3.25–5.5	50	58493	naturesQue MaxOss P, 1.0–2.0mm 2.0ml	12
58352	BEGO Semados® Tray <sup>Plus</sup> (empty), RI 3.75–5.5	56	58494	naturesQue MaxOss P, 0.25–1.0mm 0.25ml	12
58354	Drill stop Tray <sup>Plus</sup> (empty), S/SC/SCX	52	58495	naturesQue MaxOss P, 0.25–1.0mm 0.5ml	12
58356	Drill stop Tray <sup>Plus</sup> (empty), RS/RSX	55	58496	naturesQue ColTect P, 15 × 20mm	12
58357	Prosthetic kit (empty)	62	58497	naturesQue ColTect P, 20 × 30mm	12
58370	PS TiB, GH 1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (adhesive abutment)	73	58498	naturesQue ColTect P, 30 × 40mm	12
58371	PS TiB, GH 1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (adhesive abutment)	73	58499	naturesQue ColAid B, 0.1g	12
58372	PS TiB, GH 1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (adhesive abutment)	73	58500	naturesQue SemOss B, 0.25–1.0mm 0.5g; 1.0ml	12
58373	PS TiB, GH 1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (adhesive abutment)	73	58501	naturesQue SemOss B, 0.25–1.0mm 1.0g; 2.0ml	12
58374	PS TiB NH, GH 1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (adhesive abutment no Hex)	74	58502	naturesQue SemOss B, 0.25–1.0mm 0.25g; 0.5ml	12
58375	PS TiB NH, GH 1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (adhesive abutment no Hex)	74	58503	naturesQue SemOss B, 0.25–1.0mm 2.0g; 4.0ml	12
58376	PS TiB NH, GH 1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (adhesive abutment no Hex)	74	58504	naturesQue SemOss B, 1.0–2.0mm 0.5g; 1.0ml	12
58377	PS TiB NH, GH 1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (adhesive abutment no Hex)	74	58505	naturesQue SemOss B, 1.0–2.0mm 1.0g; 2.0ml	12
58386	BEGO Guide Tr (empty), RS/RSX 3.0–4.5	45	58506	naturesQue SemOss B, 1.0–2.0mm 2.0g; 4.0ml	12
58387	BEGO Guide Tray (empty), S/SC/SCX 3.25–4.5	42	58507	naturesQue ColAid P, 20 × 20mm	12
58445	PS BP, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.0 (bone shaper)	59	58515	BEGO Semados® RSX implant large-scale model	110
58446	PS BP, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (bone shapers)	59	58516*	Sub-Tec Multi <sup>Plus</sup> abutment 0°, GH 4, S/RI 3.25–3.75	100
58447	PS BP, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (bone shaper)	59	58517*	Sub-Tec Multi <sup>Plus</sup> abutment 0°, GH 4, S/RI 4.1	100
58448	PS BP, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (bone shaper)	59	58518*	Sub-Tec Multi <sup>Plus</sup> abutment 0°, GH 4, S/RI 4.5	100
58449	PS BP, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (bone shaper)	59	58866	BEGO Semados® implant, RSX <sup>Pro</sup> 3.75 L8.5	29
58488	naturesQue MaxOss P, 0.25–1.0mm 0.5ml	12	58867	BEGO Semados® implant, RSX <sup>Pro</sup> 3.75 L10	29
			58868	BEGO Semados® implant, RSX <sup>Pro</sup> 3.75 L11.5	29
			58869	BEGO Semados® implant, RSX <sup>Pro</sup> 3.75 L13	29
			58870	BEGO Semados® implant, RSX <sup>Pro</sup> 3.75 L15	29
			58871	BEGO Semados® implant, RSX <sup>Pro</sup> 4.1 L7	29
			58872	BEGO Semados® implant, RSX <sup>Pro</sup> 4.1 L8.5	29
			58873	BEGO Semados® implant, RSX <sup>Pro</sup> 4.1 L10	29
			58874	BEGO Semados® implant, RSX <sup>Pro</sup> 4.1 L11.5	29
			58875	BEGO Semados® implant, RSX <sup>Pro</sup> 4.1 L13	29
			58876	BEGO Semados® implant, RSX <sup>Pro</sup> 4.1 L15	29

**Note:** Manufacturer notes about trade names, see page 111.

\* Planned availability from November 2021

\*<sup>1</sup> Version of the BEGO Semados® RI implants, with Platform Switch design

## INDEX · PRODUCTS BY ARTICLE NUMBERS

REF	Article	Page
58877	BEGO Semados® implant, RSX <sup>Pro</sup> 4.5 L7	29
58878	BEGO Semados® implant, RSX <sup>Pro</sup> 4.5 L8.5	29
58879	BEGO Semados® implant, RSX <sup>Pro</sup> 4.5 L10	29
58880	BEGO Semados® implant, RSX <sup>Pro</sup> 4.5 L11.5	29
58881	BEGO Semados® implant, RSX <sup>Pro</sup> 4.5 L13	29
58882	BEGO Semados® implant, RSX <sup>Pro</sup> 4.5 L15	29
58883	BEGO Semados® implant, RSX <sup>Pro</sup> 5.5 L7	29
58884	BEGO Semados® implant, RSX <sup>Pro</sup> 5.5 L8.5	29
58885	BEGO Semados® implant, RSX <sup>Pro</sup> 5.5 L10	29
58886	BEGO Semados® implant, RSX <sup>Pro</sup> 5.5 L11.5	29
58887	BEGO Semados® implant, RSX <sup>Pro</sup> 5.5 L13	29
58966	BEGO Semados® implant, RS <sup>Pro</sup> 3.75 L8.5	28
58967	BEGO Semados® implant, RS <sup>Pro</sup> 3.75 L10	28
58968	BEGO Semados® implant, RS <sup>Pro</sup> 3.75 L11.5	28
58969	BEGO Semados® implant, RS <sup>Pro</sup> 3.75 L13	28
58970	BEGO Semados® implant, RS <sup>Pro</sup> 3.75 L15	28
58971	BEGO Semados® implant, RS <sup>Pro</sup> 4.1 L7	28
58972	BEGO Semados® implant, RS <sup>Pro</sup> 4.1 L8.5	28
58973	BEGO Semados® implant, RS <sup>Pro</sup> 4.1 L10	28
58974	BEGO Semados® implant, RS <sup>Pro</sup> 4.1 L11.5	28
58975	BEGO Semados® implant, RS <sup>Pro</sup> 4.1 L13	28
58976	BEGO Semados® implant, RS <sup>Pro</sup> 4.1 L15	28
58977	BEGO Semados® implant, RS <sup>Pro</sup> 4.5 L7	28
58978	BEGO Semados® implant, RS <sup>Pro</sup> 4.5 L8.5	28
58979	BEGO Semados® implant, RS <sup>Pro</sup> 4.5 L10	28
58980	BEGO Semados® implant, RS <sup>Pro</sup> 4.5 L11.5	28
58981	BEGO Semados® implant, RS <sup>Pro</sup> 4.5 L13	28
58982	BEGO Semados® implant, RS <sup>Pro</sup> 4.5 L15	28
58983	BEGO Semados® implant, RS <sup>Pro</sup> 5.5 L7	28
58984	BEGO Semados® implant, RS <sup>Pro</sup> 5.5 L8.5	28
58985	BEGO Semados® implant, RS <sup>Pro</sup> 5.5 L10	28
58986	BEGO Semados® implant, RS <sup>Pro</sup> 5.5 L11.5	28
58987	BEGO Semados® implant, RS <sup>Pro</sup> 5.5 L13	28
83538	BEGO SECURITY Implants (implant warranty)	10, 22, 26, 30, 32, 38
549316	BEG 5.DIM, S/RI 3.25–3.75 (DIM-Analog®)	94
549317	BEG 5.DIM, S/RI 4.1 (DIM-Analog®)	94
549318	BEG 5.DIM, S/RI 4.5 (DIM analog®)	94
549319	BEG 5.DIM, S/RI 5.5 (DIM analog®)	94
549320	BEG 5.DIM, RS/RSX 3.0 (DIM-Analog®)	75
549321	BPS 5.DIM, SC/SCX/RS/RSX/RI*1 3.25– 3.75 (DIM-Analog®)	75
549322	BPS 5.DIM, SC/SCX/RS/RSX/RI*1 4.1 (DIM-Analog®)	75
549323	BPS 5.DIM, SC/SCX/RS/RSX/RI*1 4.5 (DIM analog®)	75
549324	BPS 5.DIM, SC/SCX/RS/RSX/RI*1 5.5 (DIM analog®)	75
549528	BEG MU 5.DIM Multi <sup>Plus</sup> System (DIM-Analog®)	84, 102
549539	Screwdriver L24 (DYNAMIC® ABUTMENT)	67

## INDEX · PRODUCTS LISTED ALPHABETICALLY

<b>REF</b>	<b>Article</b>	<b>Page</b>
<b>A</b>		
56753	Acrylic block PS (large-scale model, scale 2:1)	<b>110</b>
<b>B</b>		
55768	Ball attachment impression set Dalbo®-PLUS	<b>88, 106</b>
549316	BEG 5.DIM, S/RI 3.25–3.75 (DIM-Analog®)	<b>94</b>
549317	BEG 5.DIM, S/RI 4.1 (DIM-Analog®)	<b>94</b>
549318	BEG 5.DIM, S/RI 4.5 (DIM-Analog®)	<b>94</b>
549319	BEG 5.DIM, S/RI 5.5 (DIM-Analog®)	<b>94</b>
549528	BEG MU 5.DIM MultiPlus System (DIM-Analog®)	<b>84, 102</b>
58065	BEGO Guide Conn, with ratchet connection, Ø4.2 (AX), RS/RSX (connector)	<b>47</b>
58051	BEGO Guide CS, (3), RS/RSX 3.0 (countersink)	<b>46</b>
58052	BEGO Guide CS, (4), RS/RSX 3.75 (countersink)	<b>46</b>
58053	BEGO Guide CS, (5), RS/RSX 4.1 (countersink)	<b>46</b>
58054	BEGO Guide CS, (6), RS/RSX 4.5 (countersink)	<b>46</b>
58066	BEGO Guide Conn, with ratchet connection, Ø4.2 (AY), RS/RSX (connector)	<b>47</b>
58067	BEGO Guide Conn, with ratchet connection, Ø4.2 (AZ), RS/RSX (connector)	<b>47</b>
58068	BEGO Guide Conn, with ratchet connection, Ø4.7 (BX), RS/RSX (connector)	<b>47</b>
58069	BEGO Guide Conn, with ratchet connection, Ø4.7 (BY), RS/RSX (connector)	<b>47</b>
58070	BEGO Guide Conn, with ratchet connection, Ø4.7 (BZ), RS/RSX (connector)	<b>47</b>
58059	BEGO Guide Conn, with contra-angle connection, Ø4.2 (AX), RS/RSX (connector)	<b>47</b>
58060	BEGO Guide Conn, with contra-angle connection, Ø4.2 (AY), RS/RSX (connector)	<b>47</b>
58061	BEGO Guide Conn, with contra-angle connection, Ø4.2 (AZ), RS/RSX (connector)	<b>47</b>
58062	BEGO Guide Conn, with contra-angle connection, Ø4.7 (BX), RS/RSX (connector)	<b>47</b>
58063	BEGO Guide Conn, with contra-angle connection, Ø4.7 (BY), RS/RSX (connector)	<b>47</b>
58064	BEGO Guide Conn, with contra-angle connection, Ø4.7 (BZ), RS/RSX (connector)	<b>47</b>
57450	BEGO Guide spoon, Ø4.2 (AX), S/SC/SCX	<b>44</b>
57451	BEGO Guide spoon, Ø4.2 (AY), S/SC/SCX	<b>44</b>
57452	BEGO Guide spoon, Ø4.2 (AZ), S/SC/SCX	<b>44</b>
57453	BEGO Guide spoon, Ø4.7 (BX), S/SC/SCX	<b>44</b>
57454	BEGO Guide spoon, Ø4.7 (BY), S/SC/SCX	<b>44</b>
57455	BEGO Guide spoon, Ø4.7 (BZ), S/SC/SCX	<b>44</b>
57713	BEGO Guide PD, Ø2.5 L18 (X2), RS/RSX (depth drill)	<b>46</b>

<b>REF</b>	<b>Article</b>	<b>Page</b>
57714	BEGO Guide pilot drill, Ø2.5 L23.5 (Y2), RS/RSX (depth drill)	<b>46</b>
57715	BEGO Guide PD, Ø2.5 L29 (Z2), RS/RSX (depth drill)	<b>46</b>
57716	BEGO Guide DD, Ø2.8 L18 (X3), RS/RSX 3.0 (depth drill)	<b>46</b>
57717	BEGO Guide DD, Ø2.8 L23.5 (Y3), RS/RSX 3.0 (depth drill)	<b>46</b>
57723	BEGO Guide DD, Ø2.8 L29 (Z3), RS/RSX 3.0 (depth drill)	<b>46</b>
57724	BEGO Guide DD, Ø3.4 L18 (X4), RS/RSX 3.75 (depth drill)	<b>46</b>
57725	BEGO Guide DD, Ø3.4 L23.5 (Y4), RS/RSX 3.75 (depth drill)	<b>46</b>
57726	BEGO Guide DD, Ø3.4 L29 (Z4), RS/RSX 3.75 (depth drill)	<b>46</b>
57727	BEGO Guide DD, Ø3.8 L18 (X5), RS/RSX 4.1 (depth drill)	<b>46</b>
57733	BEGO Guide DD, Ø3.8 L23.5 (Y5), RS/RSX 4.1 (depth drill)	<b>46</b>
57734	BEGO Guide DD, Ø3.8 L29 (Z5), RS/RSX 4.1 (depth drill)	<b>46</b>
57735	BEGO Guide DD, Ø4.1 L18 (X6), RS/RSX 4.5 (depth drill)	<b>46</b>
57736	BEGO Guide DD, Ø4.1 L23.5 (Y6), RS/RSX 4.5 (depth drill)	<b>46</b>
57737	BEGO Guide DD, Ø4.1 L29 (Z6), RS/RSX 4.5 (depth drill)	<b>46</b>
57130	BEGO Guide DS (drill sleeves)	<b>48</b>
57421	BEGO Guide tissue punches, Ø4.2 (A), S/SC/SCX/RS/RSX 3.0–3.75	<b>42, 45</b>
57422	BEGO Guide tissue punches, Ø4.7 (B), S/SC/SCX/RS/RSX 4.1–4.5	<b>42, 45</b>
57446	BEGO Guide thread tap, (3), S/SC/SCX 3.25	<b>44</b>
57447	BEGO Guide thread tap, (4), S/SC/SCX 3.75	<b>44</b>
57448	BEGO Guide thread tap, (5), S/SC/SCX 4.1	<b>44</b>
57449	BEGO Guide thread tap, (6), S/SC/SCX 4.5	<b>44</b>
57442	BEGO Guide countersink, (3), S/SC/SCX 3.25	<b>43</b>
57443	BEGO Guide countersink, (4), S/SC/SCX 3.75	<b>43</b>
57444	BEGO Guide countersink, (5), S/SC/SCX 4.1	<b>43</b>
57445	BEGO Guide countersink, (6), S/SC/SCX 4.5	<b>43</b>
57395	BEGO Guide master sleeves, Ø4.2 (A), S/SC/SCX/RS/RSX	<b>42, 45</b>
57397	BEGO Guide master sleeves, Ø4.7 (B), S/SC/SCX/RS/RSX	<b>42, 45</b>

**Note:** Manufacturer notes about trade names, see page 111.

## INDEX · PRODUCTS LISTED ALPHABETICALLY

REF	Article	Page	REF	Article	Page
57696	BEGO Guide PD, Ø2.0 L18 (X1), RS/RSX (pilot drill)	46	57413	BEGO Guide spoon, Ø2.8 (A3), S/SC/SCX 3.25	42
57697	BEGO Guide pilot drill, Ø2.0 L23.5 (Y1), RS/RSX (pilot drill)	46	57417	BEGO Guide spoon, Ø2.8 (B3), S/SC/SCX 3.25	42
57698	BEGO Guide PD, Ø2.0 L29 (Z1), RS/RSX (pilot drill)	46	57414	BEGO Guide spoon, Ø3.25 (A4), S/SC/SCX 3.75	42
57423	BEGO Guide pilot drill, Ø1.6 L18 (X1), S/SC/SCX	43	57418	BEGO Guide spoon, Ø3.25 (B4), S/SC/SCX 3.75	42
57424	BEGO Guide pilot drill, Ø1.6 L23.5 (Y1), S/SC/SCX	43	57419	BEGO Guide spoon, Ø3.65 (B5), S/SC/SCX 4.1	42
57425	BEGO Guide pilot drill, Ø1.6 L29 (Z1), S/SC/SCX	43	57420	BEGO Guide spoon, Ø4.0 (B6), S/SC/SCX 4.5	42
57458	BEGO Guide ratchet adapter for connector, S/SC/SCX	44	57426	BEGO Guide depth drill Ø2.5, L18 (X2), S/SC/SCX	43
58055	BEGO Guide ST, (3), RS/RSX 3.0 (thread tap)	47	57427	BEGO Guide depth drill, Ø2.5 L23.5 (Y2), S/SC/SCX	43
58056	BEGO Guide ST, (4), RS/RSX 3.75 (thread tap)	47	57428	BEGO Guide depth drill Ø2.5, L29 (Z2), S/SC/SCX	43
58057	BEGO Guide ST, (5), RS/RSX 4.1 (thread tap)	47	57429	BEGO Guide depth drill Ø2.8, L18 (X3), S/SC/SCX 3.25	43
57686	BEGO Guide Sp, Ø2.0 (A1), RS/RSX (reduction sleeve)	45	57430	BEGO Guide depth drill Ø2.8 L23.5 (Y3), S/SC/SCX 3.25	43
58058	BEGO Guide ST (6) RS/RSX 4.5 (thread tap)	47	57431	BEGO Guide depth drill Ø2.8, L29 (Z3), S/SC/SCX 3.25	43
57690	BEGO Guide Sp, Ø2.0 (B1), RS/RSX (reduction sleeve)	45	57432	BEGO Guide depth drill Ø3.25, L18 (X4), S/SC/SCX 3.75	43
57687	BEGO Guide Sp, Ø2.5 (A2), RS/RSX (reduction sleeve)	45	57433	BEGO Guide depth drill Ø3.25 L23.5 (Y4), S/SC/SCX 3.75	43
57691	BEGO Guide Sp, Ø2.5 (B2), RS/RSX (reduction sleeve)	45	57434	BEGO Guide depth drill Ø3.25, L29 (Z4), S/SC/SCX 3.75	43
57688	BEGO Guide Sp, Ø2.8 (A3), RS/RSX 3.0 (reduction sleeve)	45	57435	BEGO Guide depth drill Ø3.65, L18 (X5), S/SC/SCX 4.1	43
57692	BEGO Guide Sp, Ø2.8 (B3), RS/RSX 3.0 (reduction sleeve)	45	57436	BEGO Guide depth drill Ø3.65 L23.5 (Y5), S/SC/SCX 4.1	43
57689	BEGO Guide Sp, Ø3.4 (A4), RS/RSX 3.75 (reduction sleeve)	45	57437	BEGO Guide depth drill Ø3.65, L29 (Z5), S/SC/SCX 4.1	43
57693	BEGO Guide Sp, Ø3.4 (B4), RS/RSX 3.75 (reduction sleeve)	45	57438	BEGO Guide depth drill Ø4.0, L18 (X6), S/SC/SCX 4.5	43
57694	BEGO Guide Sp, Ø3.8 (B5), RS/RSX 4.1 (reduction sleeve)	45	57439	BEGO Guide depth drill Ø4.0 L23.5 (Y6), S/SC/SCX 4.5	43
57695	BEGO Guide Sp, Ø4.1 (B6), RS/RSX 4.5 (reduction sleeve)	45	57441	BEGO Guide depth drill Ø4.0, L29 (Z6), S/SC/SCX 4.5	43
57411	BEGO Guide spoon, Ø1.6 (A1), S/SC/SCX	42	57456	BEGO Guide depth stop ring connector, Ø4.2 (A), S/SC/SCX/RS/RSX	44, 47
57415	BEGO Guide spoon, Ø1.6 (B1), S/SC/SCX	42	57457	BEGO Guide depth stop ring connector, Ø4.7 (B), S/SC/SCX/RS/RSX	44, 47
57412	BEGO Guide spoon, Ø2.5 (A2), S/SC/SCX	42			
57416	BEGO Guide spoon, Ø2.5 (B2), S/SC/SCX	42			

## INDEX · PRODUCTS LISTED ALPHABETICALLY

REF	Article	Page	REF	Article	Page
58386	BEGO Guide Tr (empty), RS/RSX 3.0–4.5	45	58974	BEGO Semados® implant, RS <sup>Pro</sup> 4.1 L11.5	28
58071	BEGO Guide Tr, RS/RSX 3.0–4.5 (surgical tray)	45	58975	BEGO Semados® implant, RS <sup>Pro</sup> 4.1 L13	28
58387	BEGO Guide Tray (empty), S/SC/SCX 3.25–4.5	45	58976	BEGO Semados® implant, RS <sup>Pro</sup> 4.1 L15	28
57399	BEGO Guide Tray, S/SC/SCX 3.25–4.5	42	58977	BEGO Semados® implant, RS <sup>Pro</sup> 4.5 L7	28
57459	BEGO Guide center drill, Ø 4.2 (A), S/SC/SCX/RS/RSX 3.0–3.75	43, 46	58978	BEGO Semados® implant, RS <sup>Pro</sup> 4.5 L8.5	28
57463	BEGO Guide center drill, Ø 4.7 (B), S/SC/SCX/RS/RSX 4.1–4.5	43, 46	58979	BEGO Semados® implant, RS <sup>Pro</sup> 4.5 L10	28
57400	BEGO Guide – pilot drill, short	48	58980	BEGO Semados® implant, RS <sup>Pro</sup> 4.5 L11.5	28
57401	BEGO Guide – pilot drill, long	48	58981	BEGO Semados® implant, RS <sup>Pro</sup> 4.5 L13	28
83538	BEGO SECURITY Implants (implant warranty)	10, 22, 26, 30, 32, 38	58982	BEGO Semados® implant, RS <sup>Pro</sup> 4.5 L15	28
58515	BEGO Semados® RSX implant large-scale model	110	58983	BEGO Semados® implant, RS <sup>Pro</sup> 5.5 L7	28
57708	BEGO Semados® implant, RI 3.75 L8.5	32	578984	BEGO Semados® implant, RS <sup>Pro</sup> 5.5 L8.5	28
57709	BEGO Semados® implant, RI 3.75 L10	32	58985	BEGO Semados® implant, RS <sup>Pro</sup> 5.5 L10	28
57710	BEGO Semados® implant, RI 3.75 L11.5	32	58986	BEGO Semados® implant, RS <sup>Pro</sup> 5.5 L11.5	28
57711	BEGO Semados® implant, RI 3.75 L13	32	58987	BEGO Semados® implant, RS <sup>Pro</sup> 5.5 L13	28
57718	BEGO Semados® implant, RI 4.1 L8.5	32	57862	BEGO Semados® implant, RSX 3.0 L10	29
57719	BEGO Semados® implant, RI 4.1 L10	32	57863	BEGO Semados® implant, RSX 3.0 L11.5	29
57720	BEGO Semados® implant, RI 4.1 L11.5	32	57864	BEGO Semados® implant, RSX 3.0 L13	29
57721	BEGO Semados® implant, RI 4.1 L13	32	58866	BEGO Semados® implant, RSX <sup>Pro</sup> 3.75 L8.5	29
57728	BEGO Semados® implant, RI 4.5 L8.5	32	58867	BEGO Semados® implant, RSX <sup>Pro</sup> 3.75 L10	29
57729	BEGO Semados® implant, RI 4.5 L10	32	58868	BEGO Semados® implant, RSX <sup>Pro</sup> 3.75 L11.5	29
57730	BEGO Semados® implant, RI 4.5 L11.5	32	58869	BEGO Semados® implant, RSX <sup>Pro</sup> 3.75 L13	29
57731	BEGO Semados® implant, RI 4.5 L13	32	58870	BEGO Semados® implant, RSX <sup>Pro</sup> 3.75 L15	29
57738	BEGO Semados® implant, RI 5.5 L8.5	32	58871	BEGO Semados® implant, RSX <sup>Pro</sup> 4.1 L7	29
57739	BEGO Semados® implant, RI 5.5 L10	32	58872	BEGO Semados® implant, RSX <sup>Pro</sup> 4.1 L8.5	29
57740	BEGO Semados® implant, RI 5.5 L11.5	32	58873	BEGO Semados® implant, RSX <sup>Pro</sup> 4.1 L10	29
57741	BEGO Semados® implant, RI 5.5 L13	32	58874	BEGO Semados® implant, RSX <sup>Pro</sup> 4.1 L11.5	29
57962	BEGO Semados® implant, RS 3.0 L10	28	58875	BEGO Semados® implant, RSX <sup>Pro</sup> 4.1 L13	29
57963	BEGO Semados® implant, RS 3.0 L11.5	28	58876	BEGO Semados® implant, RSX <sup>Pro</sup> 4.1 L15	29
57964	BEGO Semados® implant, RS 3.0 L13	28	58877	BEGO Semados® implant, RSX <sup>Pro</sup> 4.5 L7	29
58330	BEGO Semados® implant, S-TG (PS) 3.75 L10	22	58878	BEGO Semados® implant, RSX <sup>Pro</sup> 4.5 L8.5	29
58331	BEGO Semados® implant, S-TG (PS) 3.75 L13	22	58879	BEGO Semados® implant, RSX <sup>Pro</sup> 4.5 L10	29
58333	BEGO Semados® implant, S-TG (PS) 4.1 L10	22	58880	BEGO Semados® implant, RSX <sup>Pro</sup> 4.5 L11.5	29
58334	BEGO Semados® implant, S-TG (PS) 4.1 L13	22	58881	BEGO Semados® implant, RSX <sup>Pro</sup> 4.5 L13	29
58966	BEGO Semados® implant, RS <sup>Pro</sup> 3.75 L8.5	28	58882	BEGO Semados® implant, RSX <sup>Pro</sup> 4.5 L15	29
58967	BEGO Semados® implant, RS <sup>Pro</sup> 3.75 L10	28	58883	BEGO Semados® implant, RSX <sup>Pro</sup> 5.5 L7	29
58968	BEGO Semados® implant, RS <sup>Pro</sup> 3.75 L11.5	28	58884	BEGO Semados® implant, RSX <sup>Pro</sup> 5.5 L8.5	29
58969	BEGO Semados® implant, RS <sup>Pro</sup> 3.75 L13	28	58885	BEGO Semados® implant, RSX <sup>Pro</sup> 5.5 L10	29
58970	BEGO Semados® implant, RS <sup>Pro</sup> 3.75 L15	28	58886	BEGO Semados® implant, RSX <sup>Pro</sup> 5.5 L11.5	29
58971	BEGO Semados® implant, RS <sup>Pro</sup> 4.1 L7	28	58887	BEGO Semados® implant, RSX <sup>Pro</sup> 5.5 L13	29
58972	BEGO Semados® implant, RS <sup>Pro</sup> 4.1 L8.5	28	57500	BEGO Semados® implant, S 3.25 L8.5	38
58973	BEGO Semados® implant, RS <sup>Pro</sup> 4.1 L10	28	57501	BEGO Semados® implant, S 3.25 L10	38
			57502	BEGO Semados® implant, S 3.25 L11.5	38
			57503	BEGO Semados® implant, S 3.25 L13	38
			57601	BEGO Semados® implant, S 3.75 L8.5	38
			57602	BEGO Semados® implant, S 3.75 L10	38

**Note:** Manufacturer notes about trade names, see page 111.

\*<sup>1</sup> Version of the BEGO Semados® RI implants, with Platform Switch design

## INDEX · PRODUCTS LISTED ALPHABETICALLY

REF	Article	Page
57603	BEGO Semados® implant, S 3.75 L11.5	38
57604	BEGO Semados® implant, S 3.75 L13	38
57840	BEGO Semados® implant, S 4.1 L7	38
57841	BEGO Semados® implant, S 4.1 L8.5	38
57842	BEGO Semados® implant, S 4.1 L10	38
57843	BEGO Semados® implant, S 4.1 L11.5	38
57844	BEGO Semados® implant, S 4.1 L13	38
57700	BEGO Semados® implant, S 4.5 L7	38
57701	BEGO Semados® implant, S 4.5 L8.5	38
57702	BEGO Semados® implant, S 4.5 L10	38
57703	BEGO Semados® implant, S 4.5 L11.5	38
57704	BEGO Semados® implant, S 4.5 L13	38
57901	BEGO Semados® implant, S 5.5 L8.5	38
57902	BEGO Semados® implant, S 5.5 L10	38
57903	BEGO Semados® implant, S 5.5 L11.5	38
57904	BEGO Semados® implant, S 5.5 L13	38
58160	BEGO Semados® implant, SC 3.25 L8.5	24
58161	BEGO Semados® implant, SC 3.25 L10	24
58162	BEGO Semados® implant, SC 3.25 L11.5	24
58163	BEGO Semados® implant, SC 3.25 L13	24
58164	BEGO Semados® implant, SC 3.25 L15	24
58165	BEGO Semados® implant, SC 3.75 L8.5	24
58166	BEGO Semados® implant, SC 3.75 L10	24
58167	BEGO Semados® implant, SC 3.75 L11.5	24
58168	BEGO Semados® implant, SC 3.75 L13	24
58169	BEGO Semados® implant, SC 3.75 L15	24
58170	BEGO Semados® implant, SC 4.1 L7	24
58171	BEGO Semados® implant, SC 4.1 L8.5	24
58172	BEGO Semados® implant, SC 4.1 L10	24
58173	BEGO Semados® implant, SC 4.1 L11.5	24
58174	BEGO Semados® implant, SC 4.1 L13	24
58175	BEGO Semados® implant, SC 4.1 L15	24
58176	BEGO Semados® implant, SC 4.5 L7	24
58177	BEGO Semados® implant, SC 4.5 L8.5	24
58178	BEGO Semados® implant, SC 4.5 L10	24
58179	BEGO Semados® implant, SC 4.5 L11.5	24
58180	BEGO Semados® implant, SC 4.5 L13	24
58181	BEGO Semados® implant, SC 4.5 L15	24
58182	BEGO Semados® implant, SC 5.5 L7	24
58183	BEGO Semados® implant, SC 5.5 L8.5	24
58184	BEGO Semados® implant, SC 5.5 L10	24
58185	BEGO Semados® implant, SC 5.5 L11.5	24
58186	BEGO Semados® implant, SC 5.5 L13	24
58260	BEGO Semados® implant, SCX 3.25 L8.5	25
58261	BEGO Semados® implant, SCX 3.25 L10	25
58262	BEGO Semados® implant, SCX 3.25 L11.5	25
58263	BEGO Semados® implant, SCX 3.25 L13	25
58264	BEGO Semados® implant, SCX 3.25 L15	25
58265	BEGO Semados® implant, SCX 3.75 L8.5	25
58266	BEGO Semados® implant, SCX 3.75 L10	25
58267	BEGO Semados® implant, SCX 3.75 L11.5	25
58268	BEGO Semados® implant, SCX 3.75 L13	25
58269	BEGO Semados® implant, SCX 3.75 L15	25
58270	BEGO Semados® implant, SCX 4.1 L7	25
58271	BEGO Semados® implant, SCX 4.1 L8.5	25
58272	BEGO Semados® implant, SCX 4.1 L10	25
58273	BEGO Semados® implant, SCX 4.1 L11.5	25
58274	BEGO Semados® implant, SCX 4.1 L13	25
58275	BEGO Semados® implant, SCX 4.1 L15	25
58276	BEGO Semados® implant, SCX 4.5 L7	25
58277	BEGO Semados® implant, SCX 4.5 L8.5	25
58278	BEGO Semados® implant, SCX 4.5 L10	25
58279	BEGO Semados® implant, SCX 4.5 L11.5	25
58280	BEGO Semados® implant, SCX 4.5 L13	25
58281	BEGO Semados® implant, SCX 4.5 L15	25
58282	BEGO Semados® implant, SCX 5.5 L7	25
58283	BEGO Semados® implant, SCX 5.5 L8.5	25
58284	BEGO Semados® implant, SCX 5.5 L10	25
58285	BEGO Semados® implant, SCX 5.5 L11.5	25
58286	BEGO Semados® implant, SCX 5.5 L13	25
55599	BEGO Semados® ratchet adapter	59, 62
58345	BEGO Semados® RI*1 demo implant	111
58322	BEGO Semados® RI*1 implant large-scale model	124
56751	BEGO Semados® RS demo implants	111
56752	BEGO Semados® RSX demo implants	111
58699	BEGO Semados® RSX demo implants 3.0	111
55543	BEGO Semados® S demo implants	111
58244	BEGO Semados® SC demo implants	111
58245	BEGO Semados® SCX demo implants	111
58242	BEGO Semados® SCX implant large-scale model	110
58346	BEGO Semados® Starter/Compact Tray <sup>Plus</sup> S/SC/SCX 3.75–4.5	50
58347	BEGO Semados® Starter/Compact Tray <sup>Plus</sup> (empty) S/SC/SCX 3.75–4.5	50
58351	BEGO Semados® Tray <sup>Plus</sup> (empty) S/SC/SCX 3.25–5.5	50
58352	BEGO Semados® Tray <sup>Plus</sup> (empty), RI 3.75–5.5	56
58350	BEGO Semados® Tray <sup>Plus</sup> (empty), RS/RSX 3.0–5.5	53
57340	BEGO Semados® Tray <sup>Plus</sup> , S/SC/SCX 3.25–5.5	50

INDEX · PRODUCTS LISTED ALPHABETICALLY

## INDEX · PRODUCTS LISTED ALPHABETICALLY

REF	Article	Page	REF	Article	Page
57612	BEGO Semados® Tray <sup>Plus</sup> , RI 3.75–5.5	56	57100	Depth drill 2.5 short, S/SC/SCX	51
57949	BEGO Semados® Tray <sup>Plus</sup> , RS/RSX 3.0–5.5	53	57927	Depth drill 2.5 long, RS/RSX	53
58349	BEGO Semados®, Starter/Compact Tray <sup>Plus</sup> (empty), RS/RSX 3.75–4.5	53	57101	Depth drill 2.5 long, S/SC/SCX	51
58348	BEGO Semados® Starter/Compact Tray <sup>Plus</sup> , RS/RSX 3.75–4.5	53	57583	Depth drill 3.2 short, RI	56
549320	BEG 5.DIM, RS/RSX 3.0 (DIM-Analog®)	75	57584	Depth drill 3.2 long, RI	56
549321	BPS 5.DIM, SC/SCX/RS/RSX/RI*1 3.25–3.75 (DIM-Analog®)	75	57585	Depth drill short, RI 3.75	57
549322	BPS 5.DIM, SC/SCX/RS/RSX/RI*1 4.1 (DIM-Analog®)	75	57587	Depth drill short, RI 4.1	57
549323	BPS 5.DIM, SC/SCX/RS/RSX/RI*1 4.5 (DIM-Analog®)	75	57589	Depth drill short, RI 4.5	57
549324	BPS 5.DIM, SC/SCX/RS/RSX/RI*1 5.5 (DIM-Analog®)	75	57591	Depth drill short, RI 5.5	57
<b>C</b>					
58191	CAD SP, S/SC/SCX/RS/RSX/RI 3.25–3.75 (scansupport)	73, 93	57928	Depth drill short, RS/RSX 3.0	54
58192	CAD SP, S/SC/SCX/RS/RSX/RI 4.1 (scansupport)	73, 93	57930	Depth drill short, RS/RSX 3.75	54
58193	CAD SP, S/SC/SCX/RS/RSX/RI 4.5 (scansupport)	73, 93	57932	Depth drill short, RS/RSX 4.1	54
58194	CAD SP, S/SC/SCX/RS/RSX/RI 5.5 (scansupport)	73, 93	57934	Depth drill short, RS/RSX 4.5	54
58255	CADP Multi <sup>Plus</sup> (CAD positioner)	85, 103	57936	Depth drill short, RS/RSX 5.5	54
57592	Countersink, RI 3.75	57	57102	Depth drill short, S/SC/SCX 3.25	51
57593	Countersink, RI 4.1	57	57104	Depth drill short, S/SC/SCX 3.75	51
57594	Countersink, RI 4.5	57	57106	Depth drill short, S/SC/SCX 4.1	51
57595	Countersink, RI 5.5	57	57108	Depth drill short, S/SC/SCX 4.5	51
57937	Countersink, RS/RSX 3.0	54	57110	Depth drill short, S/SC/SCX 5.5	51
57938	Countersink, RS/RSX 3.75	54	57586	Depth drill long, RI 3.75	57
57939	Countersink, RS/RSX 4.1	54	57588	Depth drill long, RI 4.1	57
57940	Countersink, RS/RSX 4.5	54	57590	Depth drill long, RI 4.5	57
57941	Countersink, RS/RSX 5.5	54	57929	Depth drill long, RS/RSX 3.0	54
57350	Countersink, S/SC/SCX 3.25	51	57931	Depth drill long, RS/RSX 3.75	54
57351	Countersink, S/SC/SCX 3.75	51	57933	Depth drill long, RS/RSX 4.1	54
57352	Countersink, S/SC/SCX 4.1	51	57935	Depth drill long, RS/RSX 4.5	54
57353	Countersink, S/SC/SCX 4.5	51	57103	Depth drill long, S/SC/SCX 3.25	51
57354	Countersink, S/SC/SCX 5.5	51	57105	Depth drill long, S/SC/SCX 3.75	51
<b>D</b>					
57484	DD D1, RS/RSX 3.0 (depth drill)	54	57107	Depth drill long, S/SC/SCX 4.1	51
57485	DD D1, RS/RSX 3.75 (depth drill)	54	57109	Depth drill long, S/SC/SCX 4.5	51
57486	DD D1, RS/RSX 4.1 (depth drill)	54	55746	Depth gauge, RI	59
57487	DD D1, RS/RSX 4.5 (depth drill)	54	57955	Depth gauge, RS/RSX	59
57488	DD D1, RS/RSX 5.5 (depth drill)	54	53872	Depth gauge, S/SC/SCX	59
57926	Depth drill 2.5 short, RS/RSX	53	57613	Drill module, RI 5.5	56

**Note:** Manufacturer notes about trade names, see page 111.

\*1 Version of the BEGO Semados® RI implants, with Platform Switch design

# INDEX · PRODUCTS LISTED ALPHABETICALLY

REF	Article	Page	REF	Article	Page			
57480	Drill stops, RS/RSX 5.5	55	55564	Hexagon screwdriver 1.25mm, long, contra-angle	62			
55715	Drill stops, S/SC/SCX 4.1	52	57266	Hexagon screwdriver 1.25mm XS, with ratchet connection	62			
55810	Drill stops, S/SC/SCX 4.5	52	I					
55910	Drill stops, S/SC/SCX 5.5	52	56749	IDC, RS/RSX 3.0 (adjustment instrument)	58			
55804	Drill stops, depth drill 2.5 and S/SC/SCX 3.25–3.75	52	56748	IDC, S/SC/SCX/RS/RSX/RI 3.25–5.5 (adjustment instrument)	58			
<b>E</b>								
57760	Easy-Con analog	86, 104	57950	Implant cover screw, RS/RSX 3.0	34			
57751	Easy-Con impression coping	86, 104	55505	Implant cover screw, S 3.25	40			
57753	Easy-Con instrument	87, 105	58290	Implant cover screw, SC/SCX 3.25	34			
57752	Easy-Con laboratory set	87, 105	57951	Implant cover screw, SC/SCX/RS/RSX/RI*1 3.75	34			
57754	Easy-Con production insert (black)	87, 105	57952	Implant cover screw, SC/SCX/RS/RSX/RI*1 4.1	34			
57755	Easy-Con retention insert (blue)	87, 105	57953	Implant cover screw, SC/SCX/RS/RSX/RI*1 4.5	34			
57759	Easy-Con retention insert (green)	87, 105	57954	Implant cover screw, SC/SCX/RS/RSX/RI*1 5.5	34			
57757	Easy-Con retention insert (transparent)	87, 105	55608	Implant cover screw, S/RI 3.75	40			
57756	Easy-Con retention insert (pink)	87, 105	55615	Implant cover screw, S/RI 4.1	40			
57758	Easy-Con retention insert (red)	87, 105	55616	Implant cover screw, S/RI 4.5	40			
57539	External reamer Multi <sup>Plus</sup>	85, 103	55908	Implant cover screw, S/RI 5.5	40			
55537	External reamer Universal	80, 98	57533	Insertion instrument Multi <sup>Plus</sup> abutment 0°, with ratchet connection	82, 100			
<b>F</b>								
55769	Female parts Dalbo®-PLUS	88, 106	58199	Insertion instrument Multi <sup>Plus</sup> abutment 0°, with contra-angle connection	82, 92			
<b>G</b>								
53897	Guiding wrench	58	57008	Insert tool Easy-Con/Locator®	86, 104			
<b>H</b>								
55953	Healing abutment, individual Ø 7, S/SC/SCX/RS/RSX/RI 3.25–5.5	35, 40	55831	Insert tool for implants, short, with ratchet connection	58			
57324	Healing abutment, conical, S/RI 3.25–3.75	40	56990	Insert tool for implants, short, with contra-angle connection	58			
55590	Healing abutment, Ø 4.0 L3, S/RI 3.25–3.75	40	55830	Insert tool for implants, long, with ratchet connection	58			
55591	Healing abutment, Ø 4.0 L5, S/RI 3.25–3.75	40	55832	Insert tool for implants, long, with contra-angle connection	58			
55592	Healing abutment, Ø 4.0 L7, S/RI 3.25–3.75	40	55880	Insert tool for ball attachment	88, 106			
56300	Healing abutment, Ø 4.5 L3, S/RI 3.25–4.5	40	53735	Internal reamer for gold cast-on abutment	81, 99			
56301	Healing abutment, Ø 4.5 L5, S/RI 3.25–4.5	40	57540	Internal reamer Multi <sup>Plus</sup>	85, 103			
56302	Healing abutment, Ø 4.5 L7, S/RI 3.25–4.5	40	55536	Internal reamer Universal	80, 98			
55593	Healing abutment, Ø 5.0 L3, S/RI 3.25–4.5	40	<b>M</b>					
55594	Healing abutment, Ø 5.0 L5, S/RI 3.25–4.5	40	56755	Maxilla demonstration model, RSX implants	111			
55595	Healing abutment, Ø 5.0 L7, S/RI 3.25–4.5	40	58243	Maxilla demonstration model, SCX implants	111			
56303	Healing abutment, Ø 6.0 L3, S/RI 3.25–5.5	40	56694	Model implant, 3.25	94			
56304	Healing abutment, Ø 6.0 L5, S/RI 3.25–5.5	40	56695	Model implant, S/RI 3.75	94			
56305	Healing abutment, Ø 6.0 L7, S/RI 3.25–5.5	40						
53949	Hexagon screwdriver 1.25mm, short, with ratchet connection	62						
55563	Hexagon screwdriver 1.25mm, short, contra-angle	62						
53948	Hexagon screwdriver 1.25mm, long, with ratchet connection	62						

## INDEX · PRODUCTS LISTED ALPHABETICALLY

REF	Article	Page	REF	Article	Page
56696	Model implant, S/RI 4.1	94	55863	Paralleling post, S/SC/SCX	58
56698	Model implant, S/RI 4.5	94	57581	Pilot marker, short, RI	56
56699	Model implant, S/RI 5.5	94	57481	Pilot marker, short, RS/RSX	53
57530	MultiPlus alignment aid, 20°	82, 100	57308	Pilot marker, short, S/SC/SCX	50
57531	MultiPlus alignment aid, 30°	82, 100	57582	Pilot marker, long, RI	56
57522	MultiPlus closed-tray impression, short	84, 102	57482	Pilot marker, long, RS/RSX	53
57554	MultiPlus closed-tray impression, long	84, 102	57309	Pilot marker, long, S/SC/SCX	50
57532	MultiPlus insertion splint	82, 100	55826	Prosthetic kit	62
57520	MultiPlus healing post	83, 101	58357	Prosthetic kit (empty)	62
57521	MultiPlus healing post, Mushroom	83, 101	53999	Prosthesis screw Hex 1.25mm	89, 107
57524	MultiPlus implant analog, 1 unit	84, 102	55534	Prosthesis screw Sub-Tec Universal, S/RI 3.25–4.5	107
57525	MultiPlus implant analog, 4 units	84, 102	55535	Prosthesis screw Sub-Tec Universal, S/RI 5.5	107
57523	MultiPlus open-tray impression	84, 102	57031	Prosthesis screw Sub-Tec <sup>Plus</sup>	89, 107
57526	MultiPlus titanium abutment	85, 103	58247	PS AS (selection set)	78
57538	MultiPlus Universal	85, 103	58120	PS BA, GH0, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (ball attachment abutment)	88
<b>N</b>					
58499	naturesQue ColAid B, 0.1g	12	58123	PS BA, GH0, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (ball attachment abutment)	88
58507	naturesQue ColAid P, 20 × 20mm	12	58126	PS BA, GH0, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (ball attachment abutment)	88
58496	naturesQue ColTect P, 15 × 20mm	12	58121	PS BA, GH3, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (ball attachment abutment)	88
58497	naturesQue ColTect P, 20 × 30mm	12	58124	PS BA, GH3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (ball attachment abutment)	88
58498	naturesQue ColTect P, 30 × 40mm	12	58127	PS BA, GH3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (ball attachment abutment)	88
58494	naturesQue MaxOss P, 0.25–1.0mm 0.25ml	12	58122	PS BA, GH5, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (ball attachment abutment)	88
58495	naturesQue MaxOss P, 0.25–1.0mm 0.5ml	12	58125	PS BA, GH5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (ball attachment abutment)	88
58488	naturesQue MaxOss P, 0.25–1.0mm 0.5ml	12	58128	PS BA, GH5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (ball attachment abutment)	88
58489	naturesQue MaxOss P, 0.25–1.0mm 1.0ml	12	58445	PS BP, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.0 (bone shaper)	59
58490	naturesQue MaxOss P, 0.25–1.0mm 2.0ml	12	58446	PS BP, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (bone shapers)	59
58491	naturesQue MaxOss P, 0.25–1.0mm 4.0ml	12	58447	PS BP, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (bone shaper)	59
58492	naturesQue MaxOss P, 1.0–2.0mm 1.0ml	12	58448	PS BP, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (bone shaper)	59
58493	naturesQue MaxOss P, 1.0–2.0mm 2.0ml	12	58449	PS BP, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (bone shaper)	59
58500	naturesQue SemOss B, 0.25–1.0mm 0.25g; 0.5ml	12	58250	PS CADP, RS/RSX 3.0 (CAD positioner)	72
58501	naturesQue SemOss B, 0.25–1.0mm 1.0g; 2.0ml	12	58251	PS CADP, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (CAD positioner)	73
58502	naturesQue SemOss B, 0.25–1.0mm 0.25g; 0.5ml	12			
58503	naturesQue SemOss B, 0.25–1.0mm 2.0g; 4.0ml	12			
58504	naturesQue SemOss B, 1.0–2.0mm 0.5g; 1.0ml	12			
58505	naturesQue SemOss B, 1.0–2.0mm 1.0g; 2.0ml	12			
58506	naturesQue SemOss B, 1.0–2.0mm 2.0g; 4.0ml	12			
<b>P</b>					
57598	Paralleling post, RI	58			
57956	Paralleling post, RS/RSX	58			

**Note:** Manufacturer notes about trade names, see page 111.

\*<sup>1</sup> Version of the BEGO Semados® RI implants, with Platform Switch design

## INDEX · PRODUCTS LISTED ALPHABETICALLY

REF	Article	Page	REF	Article	Page
58252	PS CADP, SC/SCX/RS/RSX/RI*1 4.1 (CAD positioner)	73	58097	PS GCO NH, SC/SCX/RS/RSX/RI*1 4.1 (gold cast-on abutment no Hex)	81
58253	PS CADP, SC/SCX/RS/RSX/RI*1 4.5 (CAD positioner)	73	58098	PS GCO NH, SC/SCX/RS/RSX/RI*1 4.5 (gold cast-on abutment no Hex)	81
58254	PS CADP, SC/SCX/RS/RSX/RI*1 5.5 (CAD positioner)	73	58099	PS GCO NH, SC/SCX/RS/RSX/RI*1 5.5 (gold cast-on abutment no Hex)	81
57773	PS CTI, SC/SCX 3.0 (impression set, closed)	75	58092	PS GCO, SC/SCX/RS/RSX/RI*1 3.25–3.75 (gold cast-on abutment)	81
58316	PS CTI, SC/SCX 3.25 (impression set, closed)	75	58093	PS GCO SC/SCX/RS/RSX/RI*1 4.1 (gold cast-on abutment)	81
57799	PS CTI, SC/SCX/RS/RSX/RI*1 3.75 (impression set, closed)	75	58094	PS GCO, SC/SCX/RS/RSX/RI*1 4.5 (gold cast-on abutment)	81
57800	PS CTI, SC/SCX/RS/RSX/RI*1 4.1 (impression set, closed)	75	57764	PS HP, Ø3.0 L3, RS/RSX 3.0 (healing abutment)	34
57801	PS CTI, SC/SCX/RS/RSX/RI*1 4.5 (impression set, closed)	75	57765	PS HP, Ø3.0 L5, RS/RSX 3.0 (healing abutment)	34
57802	PS CTI, SC/SCX/RS/RSX/RI*1 5.5 (impression set, closed)	75	57766	PS HP, Ø3.0 L7, RS/RSX 3.0 (healing abutment)	34
58130	PS Easy-Con, L1, SC/SCX/RS/RSX/RI*1 3.75 (abutment)	86	57767	PS HP, Ø4.0 L3, RS/RSX 3.0 (healing abutment)	34
58134	PS Easy-Con, L1, SC/SCX/RS/RSX/RI*1 4.1 (abutment)	86	57768	PS HP, Ø4.0 L5, RS/RSX 3.0 (healing abutment)	34
58138	PS Easy-Con, L1, SC/SCX/RS/RSX/RI*1 4.5 (abutment)	86	57769	PS HP, Ø4.0 L7, RS/RSX 3.0 (healing abutment)	34
58131	PS Easy-Con, L2, SC/SCX/RS/RSX/RI*1 3.75 (abutment)	86	57807	PS HP, Ø4.5 L3, SC/SCX/RS/RSX/RI*1 3.25–3.75 (healing abutment)	34
58135	PS Easy-Con, L2, SC/SCX/RS/RSX/RI*1 4.1 (abutment)	86	57808	PS HP, Ø4.5 L5, SC/SCX/RS/RSX/RI*1 3.25–3.75 (healing abutment)	34
58139	PS Easy-Con, L2, SC/SCX/RS/RSX/RI*1 4.5 (abutment)	86	58150	PS HP, Ø4.5 L7, SC/SCX/RS/RSX/RI*1 3.25–3.75 (healing abutment)	34
58142	PS Easy-Con, L2, SC/SCX/RS/RSX/RI*1 5.5 (abutment)	86	57809	PS HP, Ø5.0 L3, SC/SCX/RS/RSX/RI*1 4.1 (healing abutment)	34
58132	PS Easy-Con, L3, SC/SCX/RS/RSX/RI*1 3.75 (abutment)	86	57810	PS HP, Ø5.0 L5, SC/SCX/RS/RSX/RI*1 4.1 (healing abutment)	34
58136	PS Easy-Con, L3, SC/SCX/RS/RSX/RI*1 4.1 (abutment)	86	58151	PS HP, Ø5.0 L7, SC/SCX/RS/RSX/RI*1 4.1 (healing abutment)	34
58140	PS Easy-Con, L3, SC/SCX/RS/RSX/RI*1 4.5 (abutment)	86	57811	PS HP, Ø5.5 L3, SC/SCX/RS/RSX/RI*1 4.5 (healing abutment)	34
58133	PS Easy-Con, L4, SC/SCX/RS/RSX/RI*1 3.75 (abutment)	86	57812	PS HP, Ø5.5 L5, SC/SCX/RS/RSX/RI*1 4.5 (healing abutment)	34
58137	PS Easy-Con, L4, SC/SCX/RS/RSX/RI*1 4.1 (abutment)	86	58152	PS HP, Ø5.5 L7, SC/SCX/RS/RSX/RI*1 4.5 (healing abutment)	34
58141	PS Easy-Con, L4, SC/SCX/RS/RSX/RI*1 4.5 (abutment)	86	57813	PS HP, Ø6.5 L3, SC/SCX/RS/RSX/RI*1 5.5 (healing abutment)	34
58143	PS Easy-Con, L4, SC/SCX/RS/RSX/RI*1 5.5 (abutment)	86	57814	PS HP, Ø6.5 L5, SC/SCX/RS/RSX/RI*1 5.5 (healing abutment)	34
58096	PS GCO NH, SC/SCX/RS/RSX/RI*1 3.25–3.75 (gold cast-on abutment no Hex)	81	58153	PS HP, Ø6.5 L7, SC/SCX/RS/RSX/RI*1 5.5 (healing abutment)	34
			57815	PS HPW, Ø5.5 L3, SC/SCX/RS/RSX/RI*1 3.25–3.75 (healing abutment)	35
			58200	PS HPW, Ø5.5 L5, SC/SCX/RS/RSX/RI*1 3.25–3.75 (healing abutment)	35

INDEX · PRODUCTS LISTED ALPHABETICALLY

## INDEX · PRODUCTS LISTED ALPHABETICALLY

REF	Article	Page	REF	Article	Page
58201	PS HPW, Ø 5,5 L7, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (healing abutment)	35	58198*	PS Multi <sup>Plus</sup> , 0° GH 2, SC/SCX/RS/RSX/RI 4.5 (abutment)	82
57816	PS HPW, Ø 6,0 L3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (healing abutment)	35	58101	PS Multi <sup>Plus</sup> , 0° GH 3, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (abutment)	82
58202	PS HPW, Ø 6,0 L5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (healing abutment)	35	58103	PS Multi <sup>Plus</sup> , 0° GH 3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (abutment)	82
58203	PS HPW, Ø 6,0 L7, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (healing abutment)	35	58105	PS Multi <sup>Plus</sup> , 0° GH 3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (abutment)	82
57817	PS HPW, Ø 6,5 L3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (healing abutment)	35	58216*	PS Multi <sup>Plus</sup> , 0° GH 4, SC/SCX/RS/RSX/RI 3.25–3.75 (abutment)	82
58204	PS HPW, Ø 6,5 L5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (healing abutment)	35	58217*	PS Multi <sup>Plus</sup> , 0° GH 4, SC/SCX/RS/RSX/RI 4.1 (abutment)	82
58205	PS HPW, Ø 6,5 L7, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (healing abutment)	35	58218*	PS Multi <sup>Plus</sup> , 0° GH 4, SC/SCX/RS/RSX/RI 4.5 (abutment)	82
57818	PS HPW, Ø 7,0 L3, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (healing abutment)	35	58108	PS Multi <sup>Plus</sup> , 20° GH 2.3–0.6, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (abutment)	83
58206	PS HPW, Ø 7,0 L5, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (healing abutment)	35	58110	PS Multi <sup>Plus</sup> , 20° GH 2.3–0.6, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (abutment)	83
57796	PS IMPA, RS/RSX 3.0 (implant analog)	75	58112	PS Multi <sup>Plus</sup> , 20° GH 2.3–0.6, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (abutment)	83
58315	PS IMPA, SC/SCX 3.25 (implant analog)	75	58109	PS Multi <sup>Plus</sup> , 20° GH 4.0–2.3, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (abutment)	83
57819	PS IMPA, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.75 (implant analog)	75	58111	PS Multi <sup>Plus</sup> , 20° GH 4.0–2.3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (abutment)	83
57820	PS IMPA, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (implant analog)	75	58113	PS Multi <sup>Plus</sup> , 20° GH 4.0–2.3, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (abutment)	83
57821	PS IMPA, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (implant analog)	75	58116	PS Multi <sup>Plus</sup> , 30° GH 4.0–1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (abutment)	83
57822	PS IMPA, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (implant analog)	75	58117	PS Multi <sup>Plus</sup> , 30° GH 4.0–1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (abutment)	83
57778	PS ITA, RS/RSX 3.0 (temporary abutment)	76	58118	PS Multi <sup>Plus</sup> , 30° GH 4.0–1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (abutment)	83
58076	PS ITA, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (temporary abutment)	77	57774	PS CTI, RS/RSX 3.0 (impression set, open)	75
58077	PS ITA SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (temporary abutment)	77	58317	PS OTI, SC/SCX 3.25 (impression set, open)	75
58078	PS ITA SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (temporary abutment)	77	57803	PS OTI, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.75 (impression set, open)	75
58100	PS Multi <sup>Plus</sup> , 0° GH 1, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (abutment)	82	57804	PS OTI, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (impression set, open)	75
58102	PS Multi <sup>Plus</sup> , 0° GH 1, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (abutment)	82	57805	PS OTI, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (impression set, open)	75
58104	PS Multi <sup>Plus</sup> , 0° GH 1, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (abutment)	82	57806	PS OTI, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (impression set, open)	75
58196*	PS Multi <sup>Plus</sup> , 0° GH 2, SC/SCX/RS/RSX/RI 3.25–3.75 (abutment)	82	58221	PS PMB, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–5.5 (Ti-Form milling blank)	74
58197*	PS Multi <sup>Plus</sup> , 0° GH 2, SC/SCX/RS/RSX/RI 4.1 (abutment)	82			

**Note:** Manufacturer notes about trade names, see page 111.

\* Planned availability from November 2021

\*<sup>1</sup> Version of the BEGO Semados® RI implants, with Platform Switch design

## INDEX · PRODUCTS LISTED ALPHABETICALLY

REF	Article	Page	REF	Article	Page
58326	PS PMB, Ø11.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–5.5(milling blank)	74	57798	PS TiAA, 15° E GH2.5–4, RS/RSX 3.0 (solid abutment)	76
58226	PS PMB, Ø16, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–5.5 (milling blank)	74	57892	PS TiAA, 15° E GH2.5–4, SC/SCX/S/RSX/RI* <sup>1</sup> 3.25–3.75 (solid abutment)	79
58072	PS PPA, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (temporary abutment)	77	57896	PS TiAA, 15° E GH2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (solid abutment)	79
58073	PS PPA SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (temporary abutment)	77	57900	PS TiAA, 15° E GH2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	79
58074	PS PPA SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (temporary abutment)	77	57908	PS TiAA, 15° E GH2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	79
58075	PS PPA SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (temporary abutment)	77	57889	PS TiAA, 15° P GH1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (solid abutment)	79
57846	PS TiA, GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (solid abutment)	78	57893	PS TiAA, 15° P GH1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (solid abutment)	79
57848	PS TiA, GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (solid abutment)	78	57897	PS TiAA, 15° P GH1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	79
57850	PS TiA, GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	78	57905	PS TiAA, 15° P GH1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	79
57852	PS TiA, GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	78	57797	PS TiAA, 15° P GH2.5–4, RS/RSX 3.0 (solid abutment)	76
57776	PS TiA, GH2.5–4, RS/RSX 3.0 (solid abutment)	76	57890	PS TiAA, 15° P GH2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (solid abutment)	79
57847	PS TiA, GH2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (solid abutment)	78	57894	PS TiAA, 15° P GH2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (solid abutment)	79
57849	PS TiA, GH2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (solid abutment)	78	57898	PS TiAA, 15° P GH2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	79
57851	PS TiA, GH2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	78	57906	PS TiAA, 15° P GH2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	79
57853	PS TiA, GH2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	78	57911	PS TiAA, 20° E GH1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (solid abutment)	79
58088	PS TiA, conical, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (solid abutment)	78	57915	PS TiAA, 20° E GH1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (solid abutment)	79
58089	PS TiA, conical, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (solid abutment)	78	57919	PS TiAA, 20° E GH1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	79
58090	PS TiA, conical, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	78	57923	PS TiAA, 20° E GH1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	79
58091	PS TiA, conical, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	78	57912	PS TiAA, 20° E GH2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (solid abutment)	79
57891	PS TiAA, 15° E GH1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (solid abutment)	79	57916	PS TiAA, 20° E GH2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (solid abutment)	79
57895	PS TiAA, 15° E GH1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (solid abutment)	79	57920	PS TiAA, 20° E GH2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	79
57899	PS TiAA, 15° E GH1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	79	57924	PS TiAA, 20° E GH2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	79
57907	PS TiAA, 15° E GH1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	79			

INDEX · PRODUCTS LISTED ALPHABETICALLY

## INDEX · PRODUCTS LISTED ALPHABETICALLY

REF	Article	Page	REF	Article	Page
57909	PS TIAA, 20° P GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (solid abutment)	79	58370	PS TiB, GH 1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (adhesive abutment)	73
57913	PS TIAA, 20° P GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (solid abutment)	79	58371	PS TiB, GH 1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (adhesive abutment)	73
57917	PS TIAA, 20° P GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	79	58372	PS TiB, GH 1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (adhesive abutment)	73
57921	PS TIAA, 20° P GH 1–2, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	79	58373	PS TiB, GH 1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (adhesive abutment)	73
57910	PS TIAA, 20° P GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (solid abutment)	79	57781	PS TiB, RS/RSX 3.0 (adhesive abutment)	72
57914	PS TIAA, 20° P GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (solid abutment)	79	58146	PS TPA, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (temporary abutment)	77
57918	PS TIAA, 20° P GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (solid abutment)	79	58147	PS TPA SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (temporary abutment)	77
57922	PS TIAA, 20° P GH 2.5–4, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (solid abutment)	79	58148	PS TPA SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (temporary abutment)	77
57827	PS TiB NH, GH 0, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (adhesive abutment no Hex)	74	57858	PS TTiA NH, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25– 3.75 (temporary abutment no Hex)	77
57828	PS TiB NH, GH 0, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (adhesive abutment no Hex)	74	57859	PS TTiA NH, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (temporary abutment no Hex)	77
57829	PS TiB NH, GH 0, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (adhesive abutment no Hex)	74	57860	PS TTiA NH, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (temporary abutment no Hex)	77
57830	PS TiB NH, GH 0, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (adhesive abutment no Hex)	74	57861	PS TTiA NH, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (temporary abutment no Hex)	77
58374	PS TiB NH, GH 1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (adhesive abutment no Hex)	74	57854	PS TTiA, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (temporary abutment)	77
58375	PS TiB NH, GH 1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (adhesive abutment no Hex)	74	57855	PS TTiA, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (temporary abutment)	77
58376	PS TiB NH, GH 1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (adhesive abutment no Hex)	74	57856	PS TTiA, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (temporary abutment)	77
58377	PS TiB NH, GH 1.5, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (adhesive abutment no Hex)	74	57857	PS TTiA, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (temporary abutment)	77
57823	PS TiB, GH 0, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (adhesive abutment)	73	57835	PS UNI NH, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25– 3.75 (Universal no Hex abutment)	80
57824	PS TiB, GH 0, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (adhesive abutment)	73	57836	PS UNI NH, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (Universal abutment no Hex)	80
57825	PS TiB, GH 0, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (adhesive abutment)	73	57837	PS UNI NH, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.5 (Universal abutment no Hex)	80
57826	PS TiB, GH 0, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (adhesive abutment)	73	57838	PS UNI NH, SC/SCX/RS/RSX/RI* <sup>1</sup> 5.5 (Universal abutment no Hex)	80
			57993	PS UNI PScrew (prosthesis screw)	90
			57831	PS UNI, SC/SCX/RS/RSX/RI* <sup>1</sup> 3.25–3.75 (Universal abutment)	80
			57832	PS UNI, SC/SCX/RS/RSX/RI* <sup>1</sup> 4.1 (Universal abutment)	80

**Note:** Manufacturer notes about trade names, see page 111.

\* Planned availability from November 2021

\*<sup>1</sup> Version of the BEGO Semados® RI implants, with Platform Switch design

## INDEX · PRODUCTS LISTED ALPHABETICALLY

REF	Article	Page	REF	Article	Page
57833	PS UNI, SC/SCX/RS/RSX/RI*1 4.5 (Universal abutment)	80	57285	Sub-Tec CAD/CAM titanium adhesive abutment, S/RI 3.25–3.75	92
57834	PS UNI, SC/SCX/RS/RSX/RI*1 5.5 (Universal abutment)	80	57287	Sub-Tec CAD/CAM titanium adhesive abutment, S/RI 4.1	92
57782	Pscrew (prosthesis screw Ø 3.0)	89	57289	Sub-Tec CAD/CAM titanium adhesive abutment, S/RI 4.5	92
57784	Pscrew (prosthesis screw, for CAD positioner Ø 3.0)	89	57291	Sub-Tec CAD/CAM titanium adhesive abutment, S/RI 5.5	92
<b>R</b>					
55745	Radiographic template, RI implants	20	57743	Sub-Tec Easy-Con abutment, L1, S/RI 3.75–4.1	104
57959	Radiographic template, RS/RSX implants	20	57747	Sub-Tec Easy-Con abutment, L1, S/RI 4.5	104
53888	Radiographic template, S implants	20	57744	Sub-Tec Easy-Con abutment, L2, S/RI 3.75–4.1	104
58246	Radiographic template, SC/SCX implants	20	57748	Sub-Tec Easy-Con abutment, L2, S/RI 4.5	104
55799	Ratchet/torque wrench	59, 62	57745	Sub-Tec Easy-Con abutment, L3, S/RI 3.75–4.1	104
55776	Retention insert Dalbo®-PLUS	88, 106	57749	Sub-Tec Easy-Con abutment, L3, S/RI 4.5	104
<b>S</b>					
549539	Screwdriver L24 (DYNAMIC® ABUTMENT)	67	57746	Sub-Tec Easy-Con abutment, L4, S/RI 3.75–4.1	104
57535	Secondary screw MultiPlus (M1.8)	89, 107	57750	Sub-Tec Easy-Con abutment, L4, S/RI 4.5	104
57534	Secondary screw MultiPlus (M1.4)	89, 107	55873	Sub-Tec gold cast-on no Hex, S/RI 3.25–3.75	99
53952	Slot screwdriver, long with ratchet connection	62	55625	Sub-Tec gold cast-on no Hex, S/RI 4.1	99
58319	ST PMB, Ø 11.5, S/RI 3.25–5.5 (milling blank)	93	56325	Sub-Tec gold cast-on no Hex, S/RI 4.5	99
58219	ST PMB, Ø 16, S/RI 3.25–5.5 (milling blank)	93	56515	Sub-Tec gold cast-on no Hex, S/RI 5.5	99
55860	Sub-Dent closed-tray impression, S 3.25	94	55862	Sub-Tec gold cast-on, S/RI 3.25–3.75	99
55539	Sub-Dent closed-tray impression, S/RI 3.75	94	55624	Sub-Tec gold cast-on, S/RI 4.1	99
55617	Sub-Dent closed-tray impression, S/RI 4.1	94	56317	Sub-Tec gold cast-on, S/RI 4.5	99
55618	Sub-Dent closed-tray impression, S/RI 4.5	94	57631	Sub-Tec ball attachment, GH 0, S/RI 3.25–3.75	106
55551	Sub-Dent closed-tray impression, S/RI 5.5	94	57632	Sub-Tec ball attachment, GH 0, S/RI 4.1–4.5	106
55861	Sub-Dent open-tray impression, S 3.25	94	57633	Sub-Tec ball attachment, GH 3, S/RI 3.25–3.75	106
55540	Sub-Dent open-tray impression, S/RI 3.75	94	57634	Sub-Tec ball attachment, GH 3, S/RI 4.1–4.5	106
55619	Sub-Dent open-tray impression, S/RI 4.1	94	57635	Sub-Tec ball attachment, GH 5, S/RI 3.25–3.75	106
55620	Sub-Dent open-tray impression, S/RI 4.5	94	57636	Sub-Tec ball attachment, GH 5, S/RI 4.1–4.5	106
56500	Sub-Dent open-tray impression, S/RI 5.5	94	57505	Sub-Tec MultiPlus abutment 0°, GH 1, S/RI 3.25–3.75	100
57060	Sub-Tec CAD positioner, S/RI 3.25–5.5	92	57506	Sub-Tec MultiPlus abutment 0°, GH 1, S/RI 4.1	100
57656	Sub-Tec CAD/CAM TiBase L, S/RI 3.25–3.75	93	57507	Sub-Tec MultiPlus abutment 0°, GH 1, S/RI 4.5	100
57657	Sub-Tec CAD/CAM TiBase L, S/RI 4.1	93	58336*	Sub-Tec MultiPlus abutment 0°, GH 2, S/RI 3.25–3.75	100
57658	Sub-Tec CAD/CAM TiBase L, S/RI 4.5	93	58337*	Sub-Tec MultiPlus abutment 0°, GH 2, S/RI 4.1	100
57659	Sub-Tec CAD/CAM TiBase L, S/RI 5.5	93	58338*	Sub-Tec MultiPlus abutment 0°, GH 2, S/RI 4.5	100
57286	Sub-Tec CAD/CAM titanium adhesive abutment no Hex, S/RI 3.25–3.75	92	57508	Sub-Tec MultiPlus abutment 0°, GH 3, S/RI 3.25–3.75	100
57288	Sub-Tec CAD/CAM titanium adhesive abutment no Hex, S/RI 4.1	92	57509	Sub-Tec MultiPlus abutment 0°, GH 3, S/RI 4.1	100
57290	Sub-Tec CAD/CAM titanium adhesive abutment no Hex, S/RI 4.5	92	57510	Sub-Tec MultiPlus abutment 0°, GH 3, S/RI 4.5	100
57292	Sub-Tec CAD/CAM titanium adhesive abutment no Hex, S/RI 5.5	92	57511	Sub-Tec MultiPlus abutment 20°, GH 2.3–0.6, S/RI 3.25–3.75	101

## INDEX · PRODUCTS LISTED ALPHABETICALLY

REF	Article	Page	REF	Article	Page
57512	Sub-Tec Multi <sup>Plus</sup> abutment 20°, GH 2.3–0.6, S/RI 4.1	101	55525	Sub-Tec Universal, S/RI 3.25–3.75	98
57513	Sub-Tec Multi <sup>Plus</sup> abutment 20°, GH 2.3–0.6, S/RI 4.5	101	55622	Sub-Tec Universal, S/RI 4.1	98
58516*	Sub-Tec Multi <sup>Plus</sup> abutment 0°, GH 4, S/RI 3.25–3.75	100	55527	Sub-Tec Universal, S/RI 4.5	98
58517*	Sub-Tec Multi <sup>Plus</sup> abutment 0°, GH 4, S/RI 4.1	100	55529	Sub-Tec Universal, S/RI 5.5	98
58518*	Sub-Tec Multi <sup>Plus</sup> abutment 0°, GH 4, S/RI 4.5	100	57134	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 1–2, S/RI 3.25–3.75	97
57514	Sub-Tec Multi <sup>Plus</sup> abutment 20°, GH 4.0–2.3, S/RI 3.25–3.75	101	57138	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 1–2, S/RI 4.1	97
57515	Sub-Tec Multi <sup>Plus</sup> abutment 20°, GH 4.0–2.3, S/RI 4.1	101	57142	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 1–2, S/RI 4.5	97
57516	Sub-Tec Multi <sup>Plus</sup> abutment 20°, GH 4.0–2.3, S/RI 4.5	101	57146	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 1–2, S/RI 5.5	97
57517	Sub-Tec Multi <sup>Plus</sup> abutment 30°, GH 4.0–1.5, S/RI 3.25–3.75	101	57135	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 2.5–4, S/RI 3.25–3.75	97
57518	Sub-Tec Multi <sup>Plus</sup> abutment 30°, GH 4.0–1.5, S/RI 4.1	101	57139	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 2.5–4, S/RI 4.1	97
57519	Sub-Tec Multi <sup>Plus</sup> abutment 30°, GH 4.0–1.5, S/RI 4.5	101	57143	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 2.5–4, S/RI 4.5	97
57494	Sub-Tec provisional PEEK abutment, S/RI 3.25–3.75	95	57147	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° E GH 2.5–4, S/RI 5.5	97
57495	Sub-Tec provisional PEEK abutment, S/RI 4.1–4.5	95	57132	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° GH 1–2, S/RI 3.25–3.75	97
57300	Sub-Tec provisional titanium abutment no Hex, S/RI 3.25–3.75	95	57136	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° P GH 1–2, S/RI 4.1	97
57301	Sub-Tec provisional titanium abutment no Hex, S/RI 4.1	95	57140	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° P GH 1–2, S/RI 4.5	97
57302	Sub-Tec provisional titanium abutment no Hex, S/RI 4.5	95	57144	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° P GH 1–2, S/RI 5.5	97
57303	Sub-Tec provisional titanium abutment no Hex, S/RI 5.5	95	57133	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° GH 2.5–4, S/RI 3.25–3.75	97
57304	Sub-Tec provisional titanium abutment, S/RI 3.25–3.75	95	57137	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° P GH 2.5–4, S/RI 4.1	97
57305	Sub-Tec provisional titanium abutment, S/RI 4.1	95	57141	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° P GH 2.5–4, S/RI 4.5	97
57306	Sub-Tec provisional titanium abutment, S/RI 4.5	95	57145	Sub-Tec <sup>Plus</sup> titanium angulated abutment, 15° P GH 2.5–4, S/RI 5.5	97
57307	Sub-Tec provisional titanium abutment, S/RI 5.5	95	57116	Sub-Tec <sup>Plus</sup> titanium abutment, GH 1–2, S/RI 3.25–3.75	96
55951	Sub-Tec temporary abutment Ø7, S/RI 3.25–5.5	95	57120	Sub-Tec <sup>Plus</sup> titanium abutment, GH 1–2, S/RI 4.1	96
55526	Sub-Tec Universal no Hex, S/RI 3.25–3.75	98	57124	Sub-Tec <sup>Plus</sup> titanium abutment, GH 1–2, S/RI 4.5	96
55623	Sub-Tec Universal no Hex, S/RI 4.1	98	57128	Sub-Tec <sup>Plus</sup> titanium abutment, GH 1–2, S/RI 5.5	96
55528	Sub-Tec Universal no Hex, S/RI 4.5	98			
55530	Sub-Tec Universal no Hex, S/RI 5.5	98			

**Note:** Manufacturer notes about trade names, see page 111.

\* Planned availability from November 2021

\*¹ Version of the BEGO Semados® RI implants, with Platform Switch design

REF	Article	Page
57117	Sub-Tec <sup>Plus</sup> titanium abutment, GH 2.5-4, S/RI 3.25–3.75	96
57121	Sub-Tec <sup>Plus</sup> titanium abutment, GH 2.5-4, S/RI 4.1	96
57125	Sub-Tec <sup>Plus</sup> titanium abutment, GH 2.5-4, S/RI 4.5	96
57129	Sub-Tec <sup>Plus</sup> titanium abutment, GH 2.5-4,S/RI 5.5	96
<b>T</b>		
55766	Threadformer, RI 3.25	57
57615	Threadformer, RI 3.75	57
57616	Threadformer, RI 4.1	57
57617	Threadformer, RI 4.5	57
57618	Threadformer, RI 5.5	57
57619	Thread tap, RI 3.75	57
57620	Thread tap, RI 4.1	57
57621	Thread tap, RI 4.5	57
57622	Thread tap, RI 5.5	57
57943	Thread tap, RS/RSX 3.0	54
57944	Thread tap, RS/RSX 3.75	54
57945	Thread tap, RS/RSX 4.1	54
57946	Thread tap, RS/RSX 4.5	54
57947	Thread tap, RS/RSX 5.5	54
57332	Thread tap, S/SC/SCX 3.25	51
57333	Thread tap, S/SC/SCX 3.75	51
57334	Thread tap, S/SC/SCX 4.1	51
57335	Thread tap, S/SC/SCX 4.5	51
57336	Thread tap, S/SC/SCX 5.5	51
57464	TJL (training jaw) for mandible	111
57465	TJU (training jaw) for maxilla	111
55817	Trepan drill, Ø4.2 external/Ø3.7 internal	59
55815	Trepan drill, Ø5.0 external/Ø4.1 internal	59
56991	Trepan drill, Ø5.0 external/Ø4.3 internal	59
55816	Trepan drill, Ø6.0 external/Ø5.1 internal	59



# HAPPINESS



A wide range of implants  
for a variety of indications



## SEMADOS® IMPLANTS

A bright smile MADE IN GERMANY

More quality of life for patients  
with a demand-driven system

[www.bego.com](http://www.bego.com)

Partners in Progress





[www.bego.com](http://www.bego.com)



**BEGO Implant Systems GmbH & Co. KG**  
Wilhelm-Herbst-Str. 1 · 28359 Bremen, Germany  
Tel. +49 421 2028-246 · Fax +49 421 2028-265  
E-mail [info@bego-implantology.com](mailto:info@bego-implantology.com) · [www.bego.com](http://www.bego.com)

Want to always be up to date with all BEGO News?  
Register here for the BEGO newsletter: [www.bego.com/newsletter](http://www.bego.com/newsletter)



Products and services shown may not be available in all countries.

